
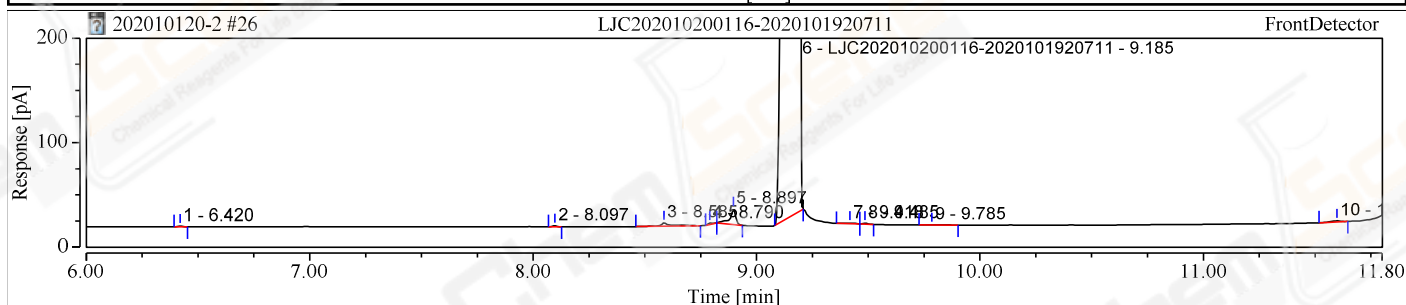


Chromatogram and Results

Injection Name: LJC202010200116-2020101920711 Vial Number: 26 Injection Type: Unknown Calibration Level: AHC008 Instrument Method: GC-FQ Processing Method: PM-LJC202010200116-2020101920711 seq.creation_operator: Ayuxp CAS NO.: 104-54-1 GC-202004	Channel: FrontDetector Wavelength: n.a. Injection Volume: 1.00 Injection Time: 20/10/2020 22:41 InstMeth.creation_time: 11/05/2020 11:09 Last update_time: 22/10/2020 10:28 Data Operator: mlill Print Operator: Ayuxp
--	---

chrom://ahyy-cm7/CM7DATA/Leyan/AHC008/Sequence/202010120-2.seq/242.smp/FrontDetector.channel/FrontDetector.chm

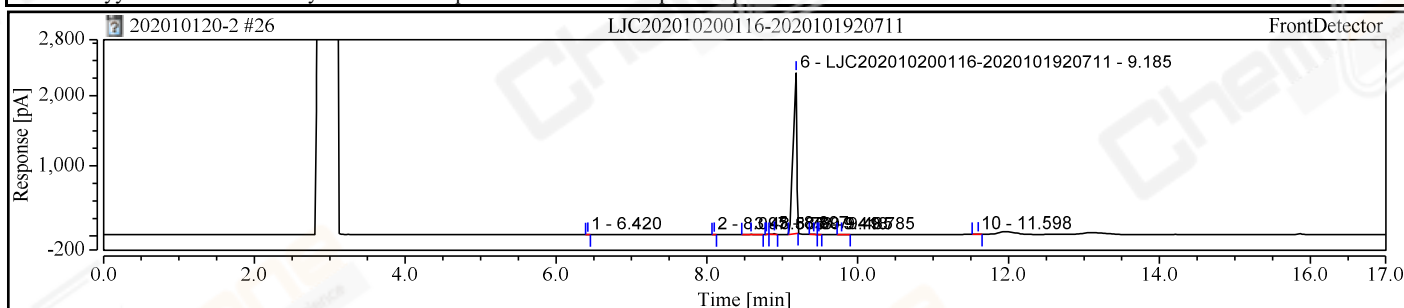

No.	Retention Time min	Area pA*min	Height pA	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	6.420	0.014	0.685	608164	51.40	1.05	0.01	
2	8.097	0.023	1.126	1004737	13.11	1.02	0.02	
3	8.585	0.189	3.313	662302	5.34	1.57	0.15	
4	8.790	0.027	1.279	1033653	2.96	1.30	0.02	
5	8.897	0.464	14.983	900856	4.14	0.68	0.36	
6	9.185	126.281	2289.091	129876	2.95	0.59	99.34	010200116-202010
7	9.418	0.023	0.514	449248	1.47	0.88	0.02	
8	9.485	0.020	0.885	1227652	6.87	1.27	0.02	
9	9.785	0.018	0.249	543624	25.51	1.81	0.01	
10	11.598	0.059	1.143	271357	n.a.	0.73	0.05	
Total:		127.117	2313.267	6831469.000	113.75			