
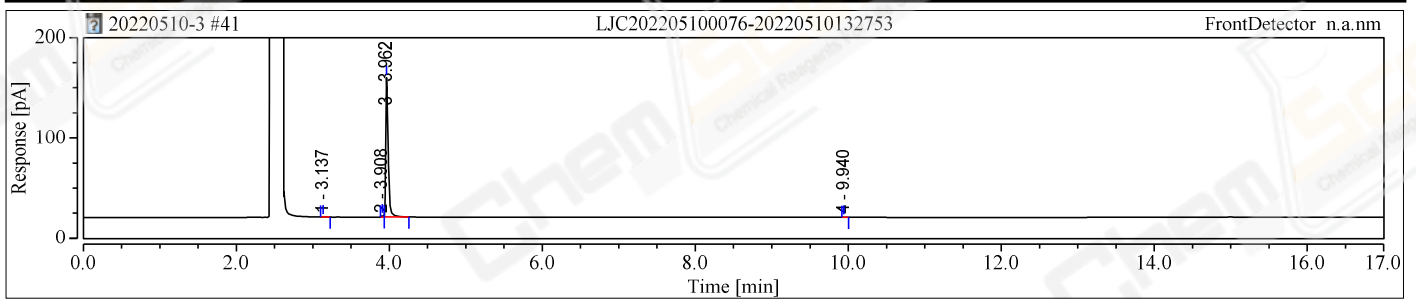


Chromatogram and Results

Sample ID: LJC202205100076-20220510132753	Comment: AH-GC004
Batch No: 1040440	Channel: FrontDetector
Vial Number: 40	Wavelength: n.a.
Injection Type: Unknown	Injection Volume: 1.00
Instrument: GC10402	Injection Time: 11/05/2022 07:07
Instrument Method: GC-FQ	InstMeth.creation_t 08/09/2020 17:08
Processing Method: PM-LJC202205100076-20220510132753	Last update_time: 11/05/2022 10:40
CAS NO.: 7051-34-5	
chrom://ahyy-cm7/CM7DATA/Leyan/GC10402/Sequence/20220510-3.seq/484.smp/FrontDetector.channel/FrontDetector.chm	

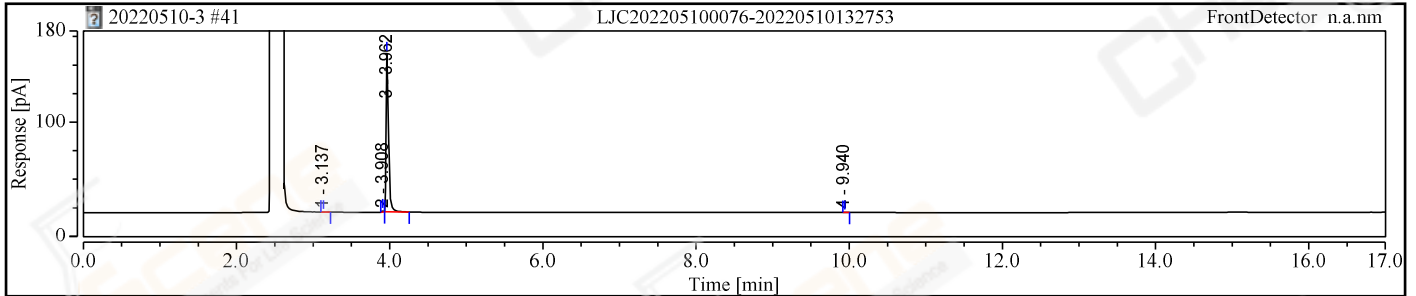

No.	Retention Time min	Area pA*min	Height pA	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	3.137	0.009	0.158	22355	12.25	1.67	0.164	
2	3.908	0.030	1.168	137858	1.05	1.12	0.565	
3	3.962	5.318	138.514	70246	110.96	1.97	99.188	
4	9.940	0.004	0.112	687104	n.a.	1.79	0.083	
Total:		5.362	139.952		124.25			