
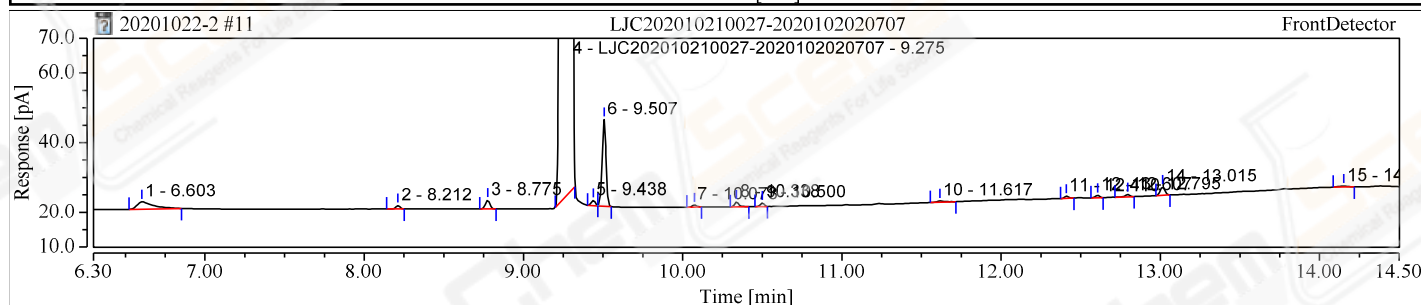


## Chromatogram and Results

Injection Name: LJC202010210027-2020102020707	Channel: FrontDetector
Vial Number: 11	Wavelength: n.a.
Injection Type: Unknown	Injection Volume: 1.00
Calibration Level: AHC008	Injection Time: 22/10/2020 19:17
Instrument Method: GC-FQ-DB-624	InstMeth.creation_time: 11/05/2020 11:09
Processing Method: PM-LJC202010210027-2020102020707	Last update_time: 23/10/2020 10:52
seq.creation_operator: Ayuxp	Data Operator: mlill
CAS NO.: 108-93-0	

chrom://ahyy-cm7/CM7DATA/Leyan/AHC008/Sequence/20201022-2.seq/314.smp/FrontDetector.channel/FrontDetector.chm

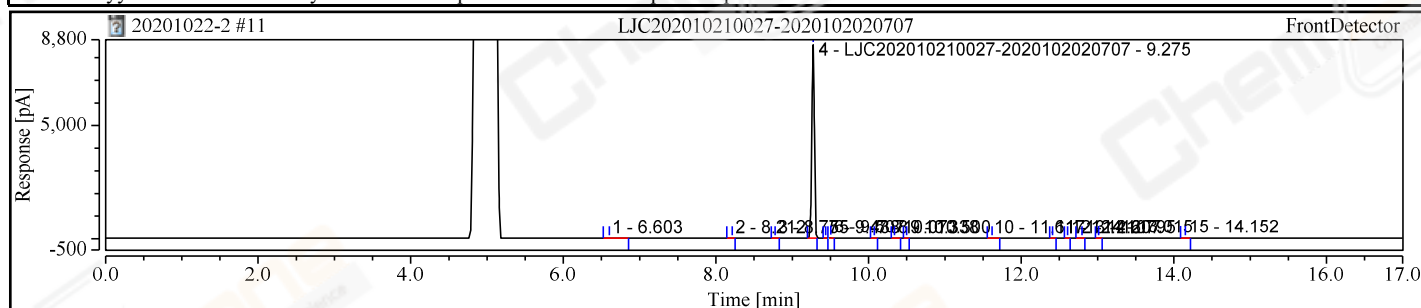

No.	Retention Time min	Area pA*min	Height pA	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	6.603	0.250	2.104	26687	15.30	2.28	0.08	
2	8.212	0.031	0.991	456818	11.27	0.97	0.01	
3	8.775	0.081	2.533	467439	8.92	1.02	0.02	
4	9.275	324.725	8542.370	372360	2.97	0.89	99.58	010210027-202010
5	9.438	0.043	1.454	589682	1.45	n.a.	0.01	
6	9.507	0.709	24.932	709825	12.78	0.98	0.22	
7	10.073	0.017	0.602	855724	5.98	1.06	0.01	
8	10.338	0.042	1.383	843361	3.64	1.47	0.01	
9	10.500	0.029	1.041	921138	20.69	0.97	0.01	
10	11.617	0.022	0.392	524548	14.30	1.57	0.01	
11	12.410	0.019	0.644	1124677	4.11	1.15	0.01	
12	12.607	0.021	0.683	1060853	3.73	0.91	0.01	
13	12.795	0.023	0.651	965541	4.17	0.87	0.01	
14	13.015	0.080	2.401	946944	16.15	1.02	0.02	
15	14.152	0.019	0.275	420576	n.a.	1.03	0.01	
<b>Total:</b>		326.111	8582.458	10286173.000	125.45			