
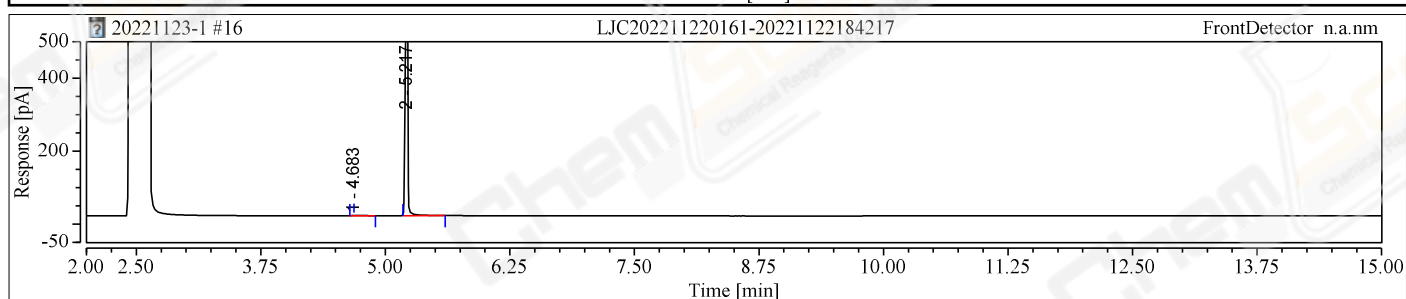


Chromatogram and Results

CAS NO.:	74181-34-3	Comment:	AH-GC003
Batch No:	1064129	Channel:	FrontDetector
Vial Number:	42	Wavelength:	n.a.
Injection Type:	Unknown	Injection Volume:	1.00
Instrument:	GC10402	Injection Time:	23/11/2022 19:30
Instrument Method:	GC-FQ	InstMeth.creation_t	11/05/2020 11:09
Processing Method:	PM-LJC202211220161-20221122184217	Last update_time:	24/11/2022 10:55
seq.creation_operator	Myuxp		
chrom://ahyy-cm7/CM7DATA/Leyan/GC10402/Sequence/2022/202211/20221123-1.seq/647.smp/FrontDetector.channel/FrontDetector.chm			

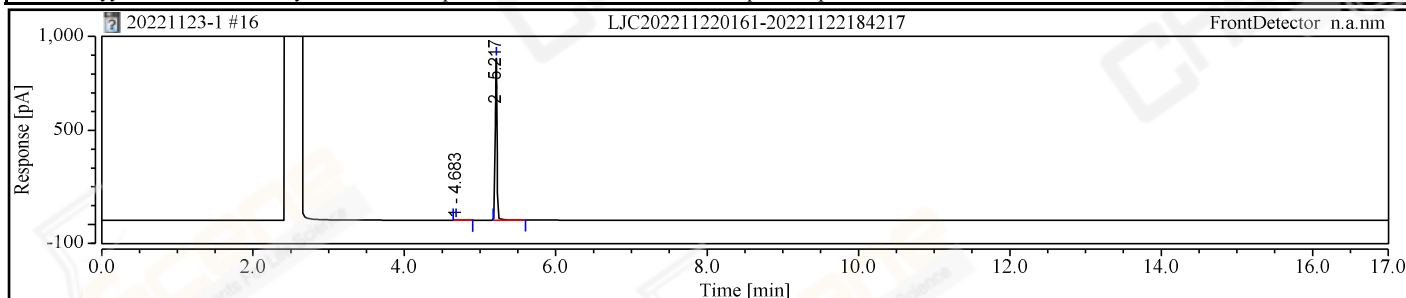

No.	Retention Time min	Area pA*min	Height pA	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	4.683	0.123	1.055	10132	4.63	3.36	0.538	
2	5.217	22.717	859.630	219824	n.a.	0.77	99.462	
Total:		22.840	860.685		4.63			