
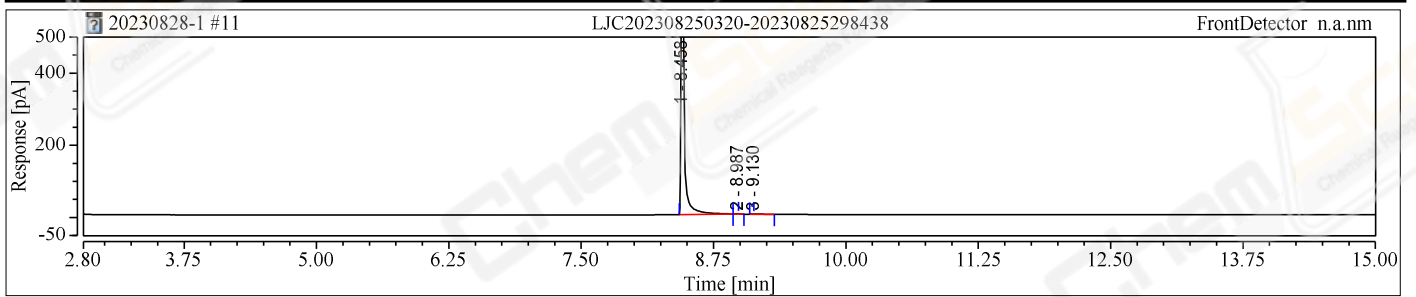


Chromatogram and Results

CAS NO.:	4730-54-5	Comment:	AH-GC039
Batch No:		Channel:	FrontDetector
Vial Number:	9	Wavelength:	n.a.
Injection Type:	Unknown	Injection Volume:	1.00
Instrument:	GC10402	Injection Time:	28/08/2023 13:29
Instrument Method:	GC-FQ	InstMeth.creation_t	11/05/2020 11:09
Processing Method:	LJC202308250320-20230825298438	Last update_time:	28/08/2023 16:47
seq.creation_operator	Yuxiaoping		
chrom://ahyy-cm7/CM7DATA/Leyan/GC10402/Sequence/2023/202308/20230828-1.seq/306.smp/FrontDetector.channel/FrontDetector.chm			

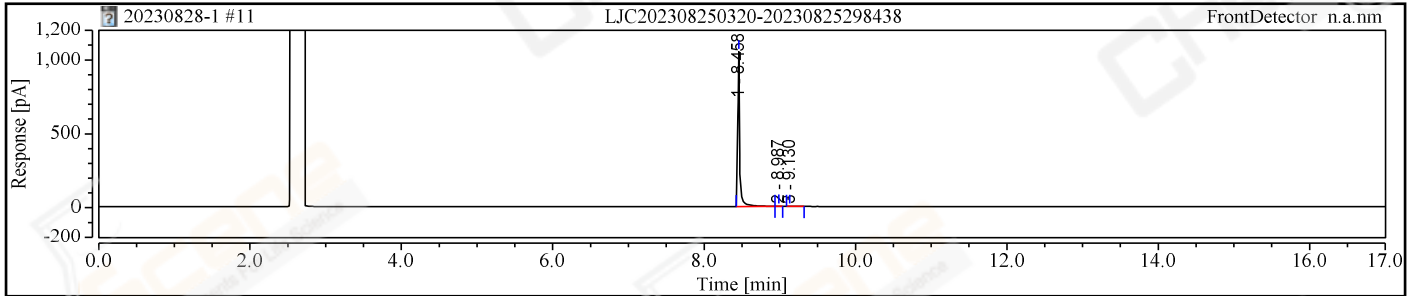

No.	Retention Time min	Area pA*min	Height pA	Plates (EP)	Resolution (EP)	Asymmetry (EP)	Rel.Area %	Peak Name
1	8.458	30.326	1048.520	774500	12.28	1.39	99.594	
2	8.987	0.035	0.955	564634	1.17	0.91	0.116	
3	9.130	0.088	0.741	34237	n.a.	3.11	0.289	
Total:		30.450	1050.216		13.45			