


| | | | |
|-----------------|--------------------------|-----------------------|----------------------|
| Catalog No | : CS-W007388 Batch#43212 | Date | : 2017-6-14 10:13:15 |
| Sample Name | : 1021713 | Data Acquisition Time | : 2017-6-13 18:32:01 |
| Instrument Name | : CLARUS 600 | Channel | : A |
| Rack/Vial | : 0/18 | Operator | : manager |
| Sample Amount | : 1.000000 | Dilution Factor | : 1.000000 |
| Cycle | : 1 | | |

Result File :
Sequence File : D:\sequence\170613-2.seq

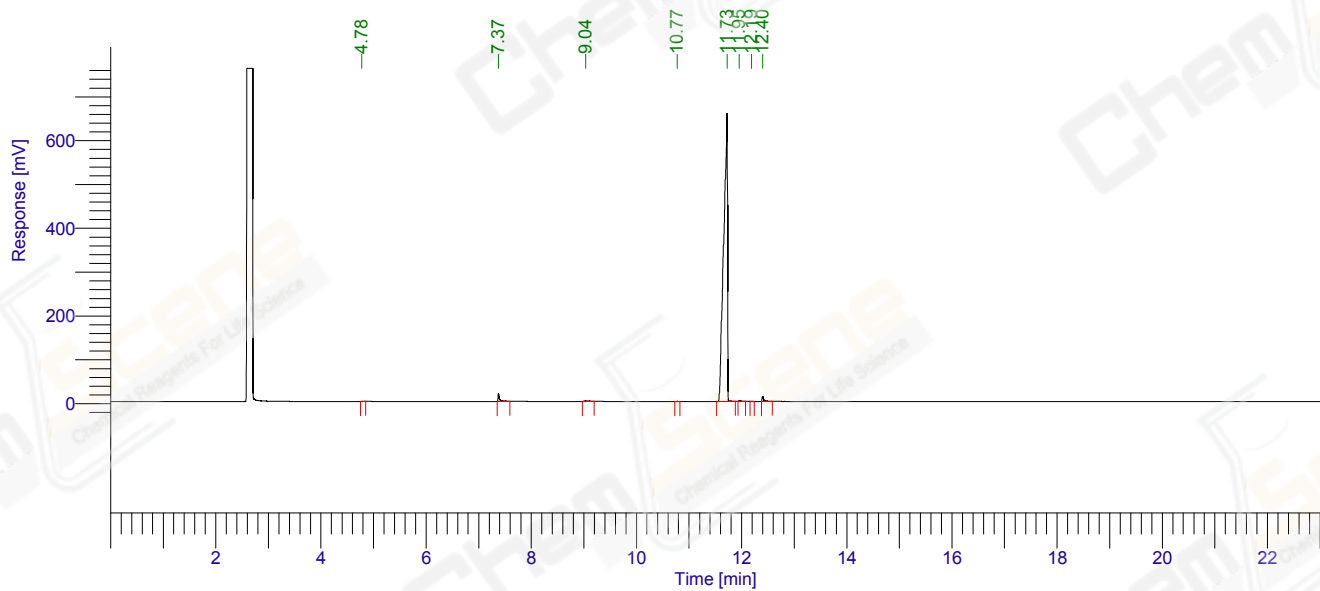

Area Percent Report

| Peak # | Component Name | Time [min] | Area [UV*sec] | Area Percent [%] |
|--------|----------------|------------|---------------|------------------|
| 1 | | 4.778 | 1535.87 | 0.0453 |
| 2 | | 7.374 | 36885.94 | 1.0880 |
| 3 | | 9.035 | 9326.11 | 0.2751 |
| 4 | | 10.774 | 514.75 | 0.0152 |
| 5 | | 11.726 | 3314437.34 | 97.7650 |
| 6 | | 11.954 | 4650.46 | 0.1372 |
| 7 | | 12.190 | 419.78 | 0.0124 |
| 8 | | 12.400 | 22438.34 | 0.6619 |
| | | | 3390208.57 | 100.0000 |

Missing Component Report
Component Expected Retention (Calibration File)

All components were found