


Software Version : 6.3.1.0504 Date : 2017-6-14 10:13:15
 Sample Name : 1021713 Data Acquisition Time : 2017-6-13 18:32:01
 Instrument Name : CLARUS 600 Channel : A
 Rack/Vial : 0/18 Operator : manager
 Sample Amount : 1.000000 Dilution Factor : 1.000000
 Cycle : 1
 Catalog No : CS-W007388 Batch# La0607037

Result File :
 Sequence File : D:\sequence\170613-2.seq

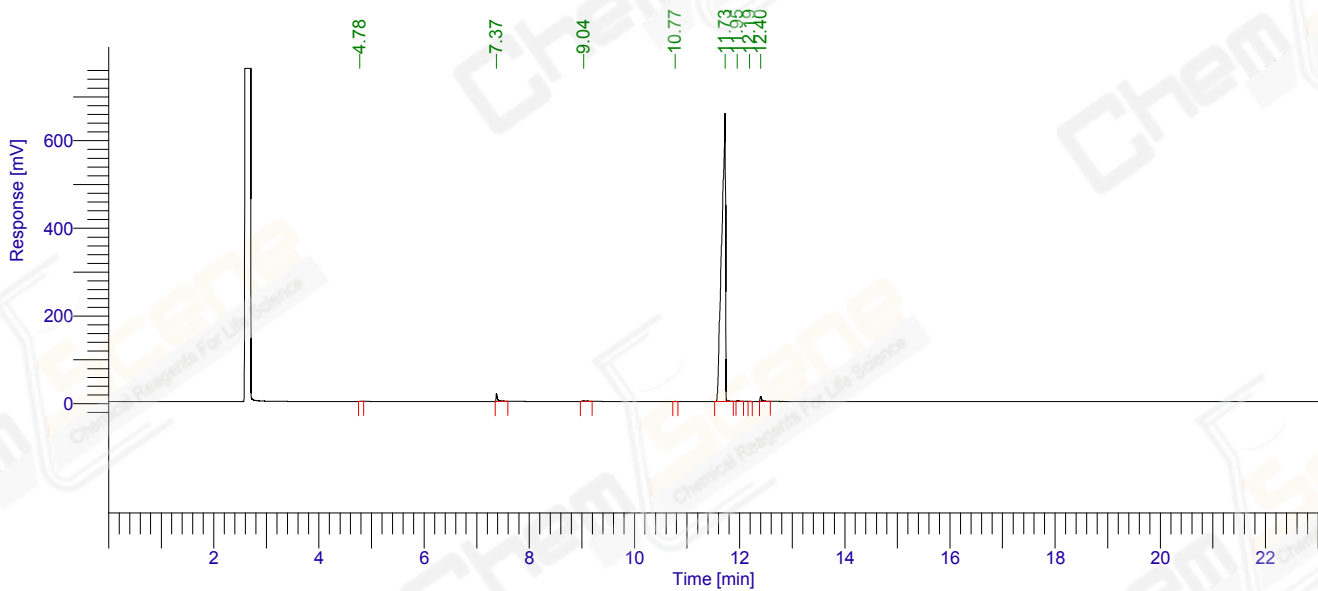

Area Percent Report

Peak #	Component Name	Time [min]	Area [UV*sec]	Area Percent [%]
1		4.778	1535.87	0.0453
2		7.374	36885.94	1.0880
3		9.035	9326.11	0.2751
4		10.774	514.75	0.0152
5		11.726	3314437.34	97.7650
6		11.954	4650.46	0.1372
7		12.190	419.78	0.0124
8		12.400	22438.34	0.6619
			3390208.57	100.0000

Missing Component Report
 Component Expected Retention (Calibration File)

All components were found