
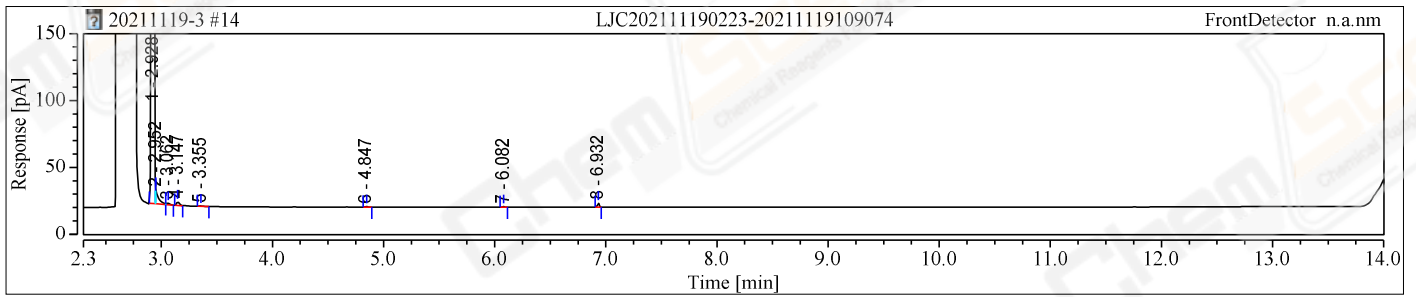


## Chromatogram and Results

CAS NO.:	16545-68-9	Channel:	FrontDetector
Vial Number:	14	Wavelength:	n.a.
Injection Type:	Unknown	Injection Volume:	1.00
Instrument:	AHC008	Injection Time:	20/11/2021 01:39
Instrument Method:	GC-FQ	InstMeth.creation_time:	11/05/2020 11:09
Processing Method:	PM-LJC202111190223-20211119109074	Last update_time:	20/11/2021 14:31
seq.creation_operator	Azouyl	Data Operator:	Mzhaodh
Comment	1129774 GC-202004	Print Operator:	Azouyl
chrom://ahyy-cm7/CM7DATA/Leyan/AHC008/Sequence/2021/202111/20211119-3.seq/461.smp/FrontDetector.channel/FrontDetector.chm			

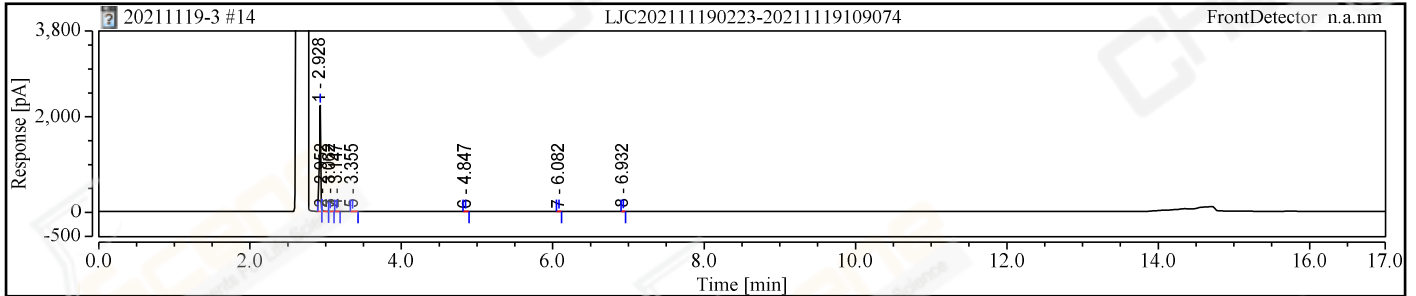

No.	Retention Time min	Area pA*min	Height pA	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	2.928	42.628	2215.736	140019	0.45	0.79	98.779	
2	2.952	0.306	10.842	26481	1.72	n.a.	0.709	
3	3.062	0.039	1.192	48588	1.64	n.a.	0.089	
4	3.147	0.082	2.777	68102	4.61	1.44	0.190	
5	3.355	0.011	0.363	101528	39.54	1.71	0.026	
6	4.847	0.013	0.589	338077	37.78	1.00	0.030	
7	6.082	0.013	0.665	576364	26.79	1.07	0.031	
8	6.932	0.063	3.233	779610	n.a.	0.99	0.147	
Total:		43.155	2235.396		112.52			