
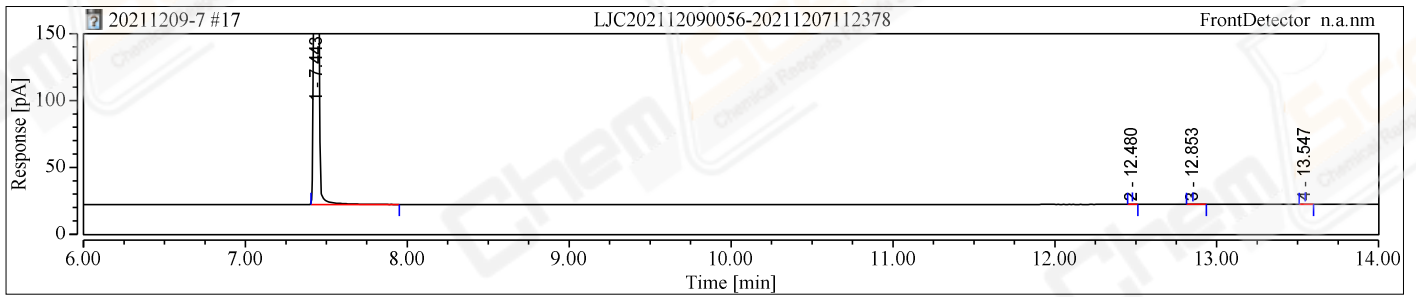


Chromatogram and Results

CAS NO.:	54087-03-5	Channel:	FrontDetector
Vial Number:	15	Wavelength:	n.a.
Injection Type:	Unknown	Injection Volume:	1.00
Instrument:	AHC008	Injection Time:	10/12/2021 02:42
Instrument Method:	GC-FQ	InstMeth.creation_time:	11/05/2020 11:09
Processing Method:	PM-LJC202112090056-20211207112378	Last update_time:	10/12/2021 12:57
seq.creation_operator	Myuxp	Data Operator:	Myuxp
Comment	GC-202004 1062792	Print Operator:	Myuxp
chrom://ahyy-cm7/CM7DATA/Leyan/AHC008/Sequence/2021/202112/20211209-7.seq/918.smp/FrontDetector.channel/FrontDetector.chm			

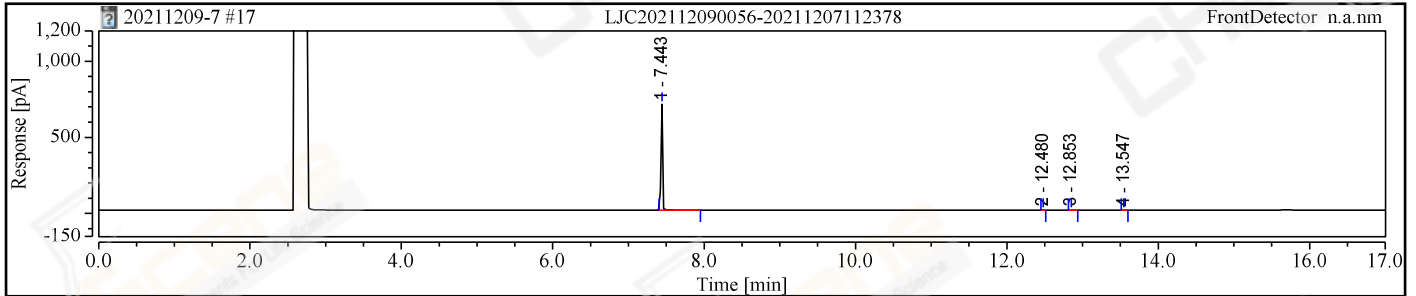

No.	Retention Time min	Area pA*min	Height pA	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	7.443	17.043	696.181	561431	120.44	0.81	99.953	
2	12.480	0.002	0.058	1292979	7.06	1.08	0.011	
3	12.853	0.003	0.059	690602	12.22	1.48	0.018	
4	13.547	0.003	0.075	1103362	n.a.	1.24	0.017	
Total:		17.051	696.374		139.72			