
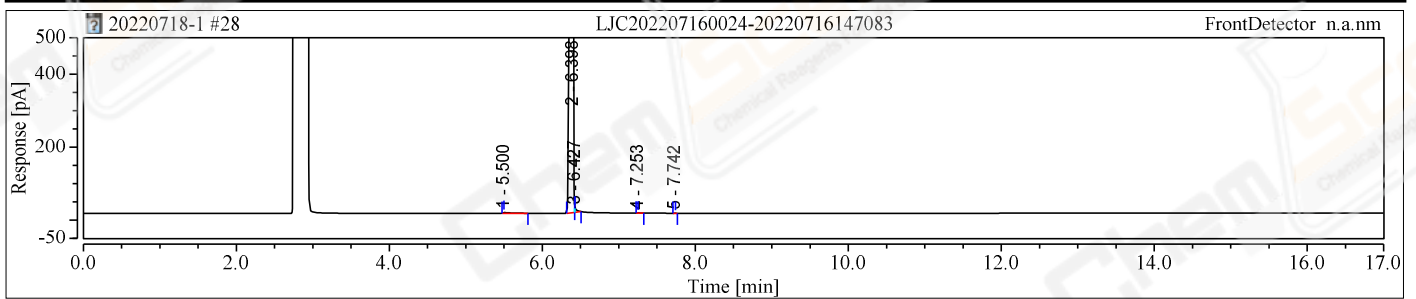


Chromatogram and Results

Sample ID:	LJC202207160024-20220716147083	Comment:	AH-GC003
CAS NO.:	56423-63-3	Channel:	FrontDetector
Vial Number:	66	Wavelength:	n.a.
Injection Type:	Unknown	Injection Volume:	1.00
Instrument:	GC10402	Injection Time:	19/07/2022 02:12
Instrument Method:	GC-FQ	InstMeth.creation_t	11/05/2020 11:09
Processing Method:	PM-LJC202207160024-20220716147083	Last update_time:	19/07/2022 11:09
seq.creation_operator	Myuxp		
chrom://ahyy-cm7/CM7DATA/Leyan/GC10402/Sequence/2022/202207/20220718-1.seq/854.smp/FrontDetector.channel/FrontDetector.chm			

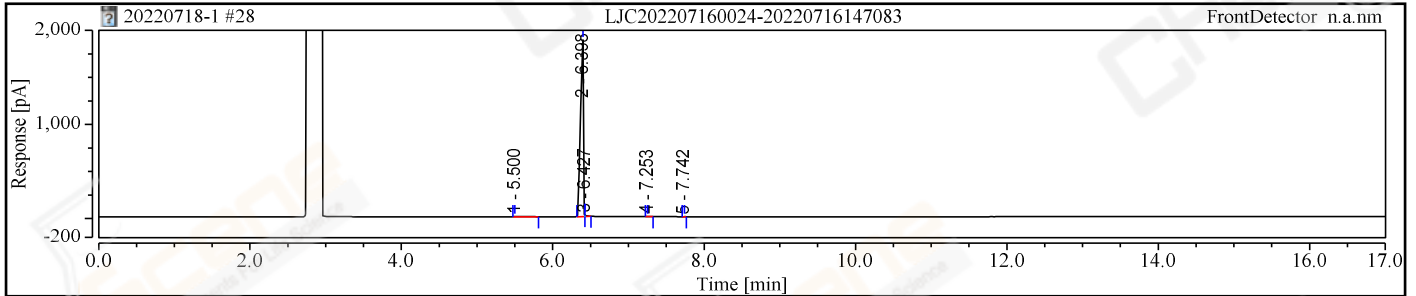

No.	Retention Time min	Area pA*min	Height pA	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	5.500	0.319	2.803	35749	9.07	6.90	0.376	
2	6.398	83.990	1879.386	98200	0.65	0.63	99.162	
3	6.427	0.361	11.570	23684966	25.29	n.a.	0.426	
4	7.253	0.026	0.621	233093	10.57	1.94	0.030	
5	7.742	0.004	0.212	918568	n.a.	0.99	0.005	
Total:		84.699	1894.592		45.58			