
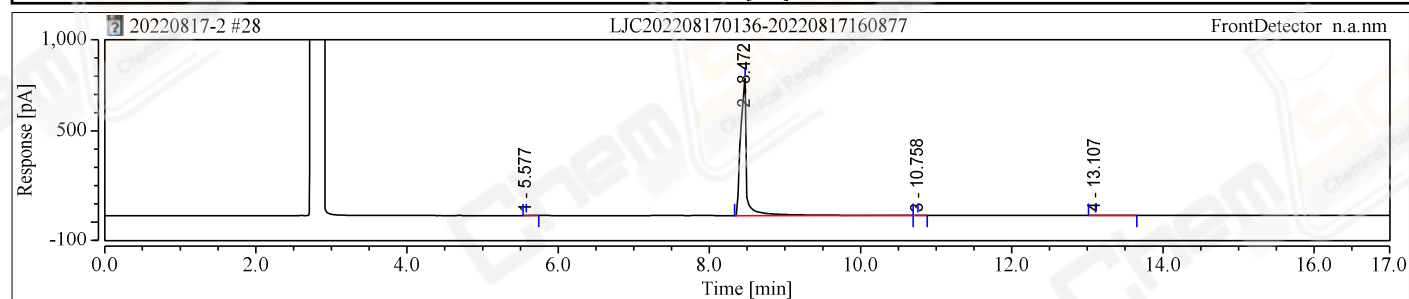


Chromatogram and Results

CAS NO.: 67-47-0	Comment:
Batch No: 1039583	Channel: FrontDetector
Vial Number: 23	Wavelength: n.a.
Injection Type: Unknown	Injection Volume: 1.00
Instrument: GC10402	Injection Time: 17/08/2022 22:16
Instrument Method: GC-FQ	InstMeth.creation_t 11/05/2020 11:09
Processing Method: PM-LJC202208170136-20220817160877	Last update_time: 18/08/2022 10:23
seq.creation_operator Myuxp	
chrom://ahyy-cm7/CM7DATA/Leyan/GC10402/Sequence/2022/202208/20220817-2.seq/118.smp/FrontDetector.channel/FrontDetector.chm	

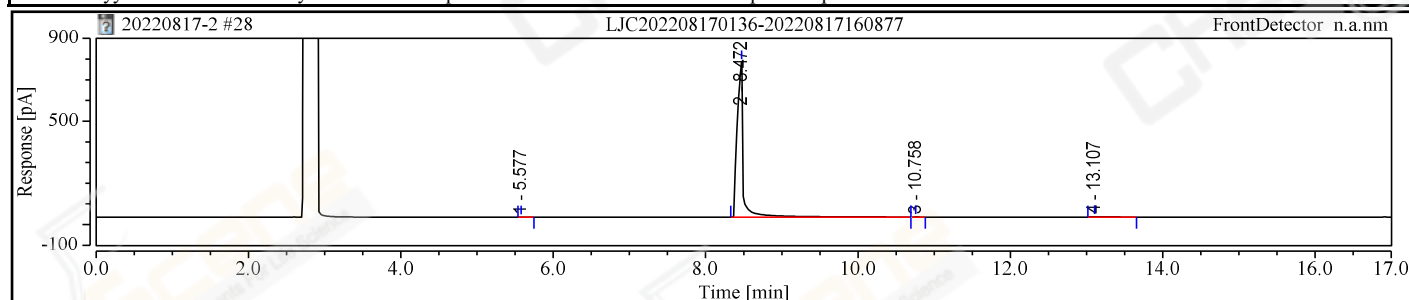

No.	Retention Time min	Area pA*min	Height pA	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	5.577	0.032	0.335	37359	24.71	3.10	0.046	
2	8.472	68.792	750.615	81190	20.20	0.94	99.574	
3	10.758	0.038	0.469	160326	7.15	n.a.	0.055	
4	13.107	0.224	0.722	9110	n.a.	3.66	0.325	
Total:		69.086	752.141		52.06			