
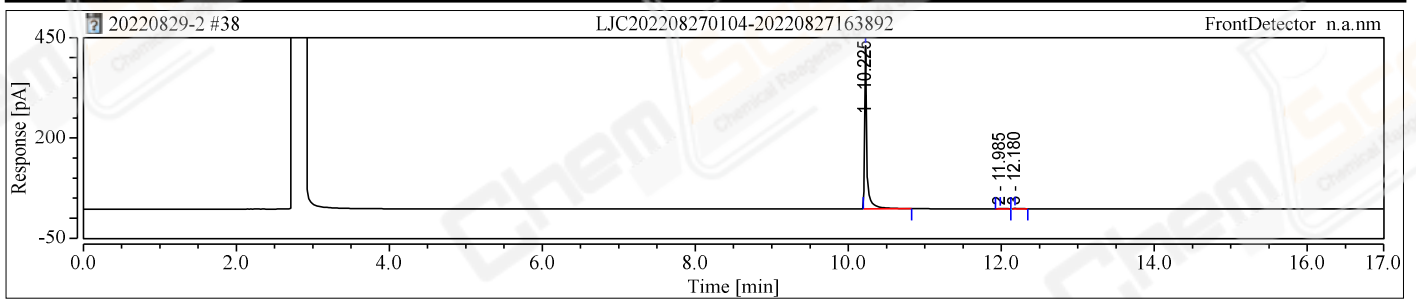


Chromatogram and Results

CAS NO.:	101935-40-4	Comment:	AH-GC003
Batch No:	1063019	Channel:	FrontDetector
Vial Number:	17	Wavelength:	n.a.
Injection Type:	Unknown	Injection Volume:	1.00
Instrument:	GC10402	Injection Time:	30/08/2022 04:01
Instrument Method:	GC-FQ	InstMeth.creation_t	11/05/2020 11:09
Processing Method:	PM-LJC202208270104-20220827163892	Last update_time:	30/08/2022 10:58
seq.creation_operator	Myuxp		
chrom://ahyy-cm7/CM7DATA/Leyan/GC10402/Sequence/2022/202208/20220829-2.seq/314.smp/FrontDetector.channel/FrontDetector.chm			

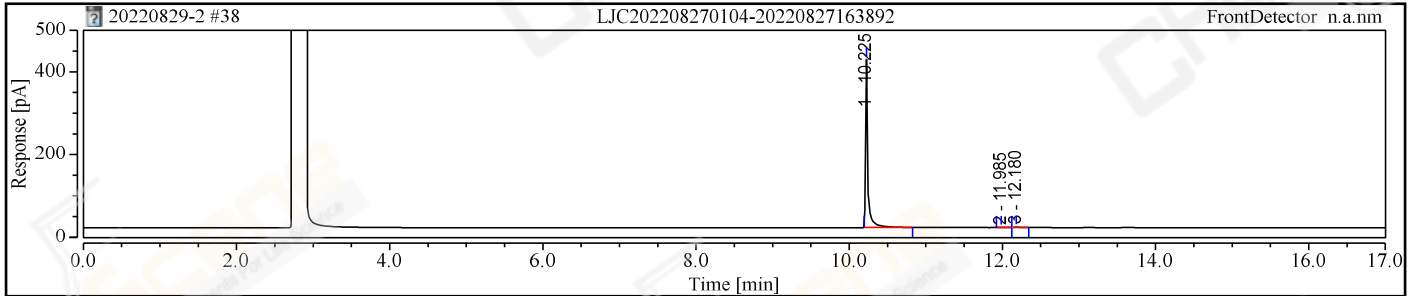

No.	Retention Time min	Area pA*min	Height pA	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	10.225	13.393	406.371	1131740	14.39	2.04	99.077	
2	11.985	0.044	0.374	54067	1.25	n.a.	0.327	
3	12.180	0.081	0.987	215276	n.a.	n.a.	0.596	
Total:		13.518	407.731		15.64			