
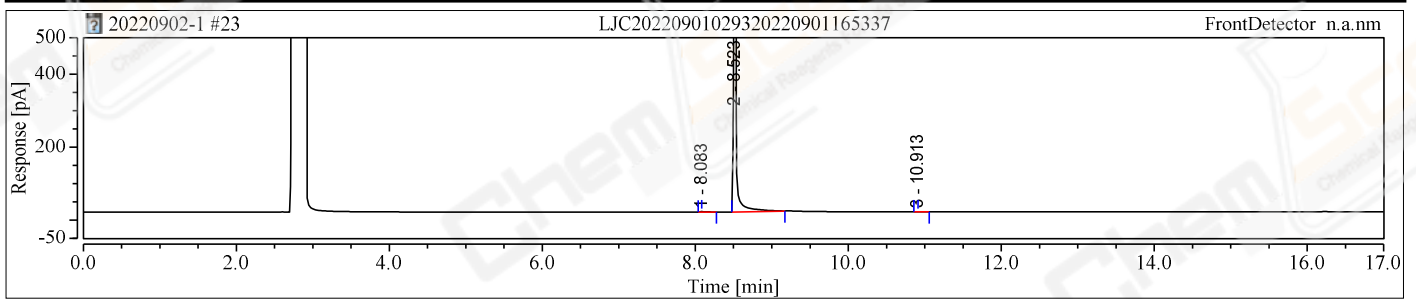


## Chromatogram and Results

Sample ID: LJC2022	Comment: AH-GC003
CAS NO.: 14572-89-5	Channel: FrontDetector
Vial Number: 8	Wavelength: n.a.
Injection Type: Unknown	Injection Volume: 1.00
Instrument: GC10402	Injection Time: 03/09/2022 00:04
Instrument Method: GC-FQ	InstMeth.creation_t 11/05/2020 11:09
Processing Method: PM-LJC2022	Last update_time: 05/09/2022 10:01
seq.creation_operator: Myuxp	
chrom://ahyy-cm7/CM7DATA/Leyan/GC10402/Sequence/2022/202209/20220902-1.seq/952.smp/FrontDetector.channel/FrontDetector.chm	

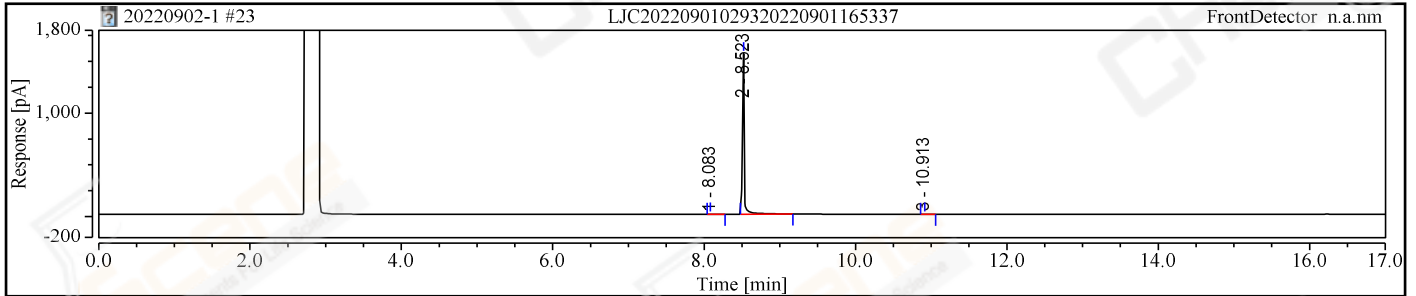

No.	Retention Time min	Area pA*min	Height pA	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	8.083	0.115	1.215	54181	4.75	2.77	0.245	
2	8.523	47.033	1551.850	544654	26.60	0.77	99.640	
3	10.913	0.055	0.592	106875	n.a.	2.31	0.116	
Total:		47.203	1553.658		31.35			