
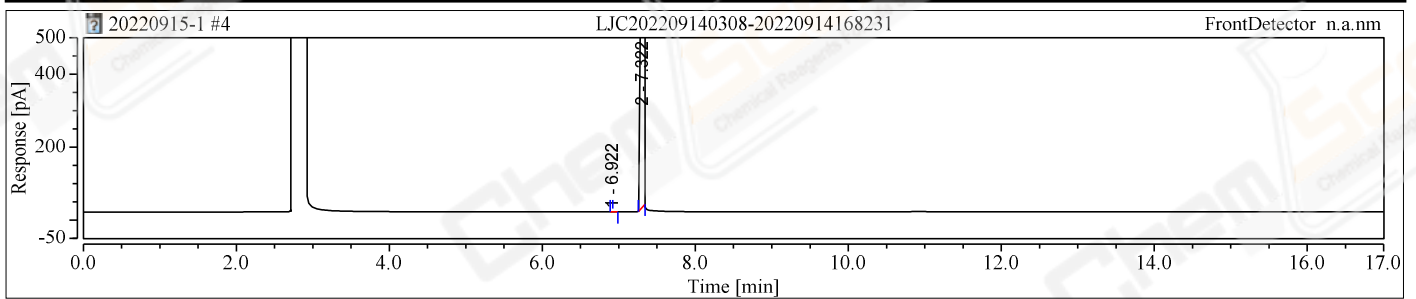


Chromatogram and Results

CAS NO.:	544-40-1	Comment:	AH-GC003
Batch No:		Channel:	FrontDetector
Vial Number:	4	Wavelength:	n.a.
Injection Type:	Unknown	Injection Volume:	1.00
Instrument:	GC10402	Injection Time:	15/09/2022 11:13
Instrument Method:	GC-FQ	InstMeth.creation_t	11/05/2020 11:09
Processing Method:	PM-LJC202209140308-20220914168231	Last update_time:	16/09/2022 09:11
seq.creation_operator	Myangby		
chrom://ahyy-cm7/CM7DATA/Leyan/GC10402/Sequence/2022/202209/20220915-1.seq/935.smp/FrontDetector.channel/FrontDetector.chm			

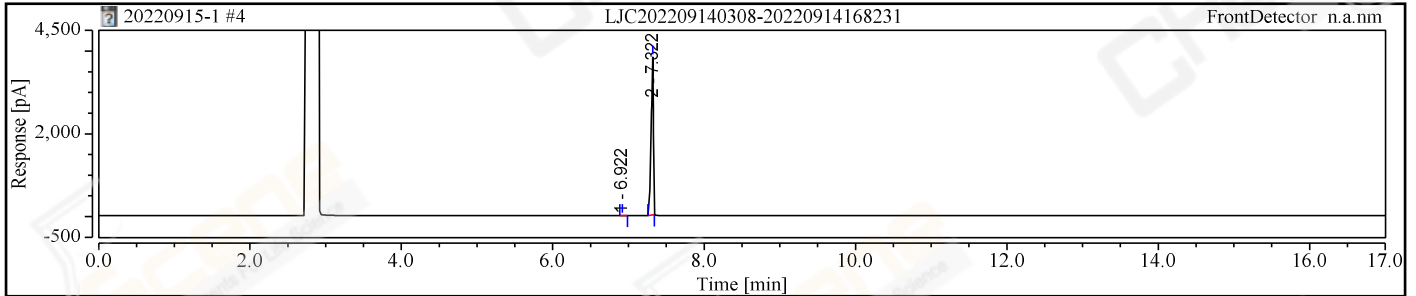

No.	Retention Time min	Area pA*min	Height pA	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	6.922	0.029	0.529	106176	5.57	1.48	0.023	
2	7.322	126.198	3812.212	250350	n.a.	0.65	99.977	
Total:		126.227	3812.741		5.57			