
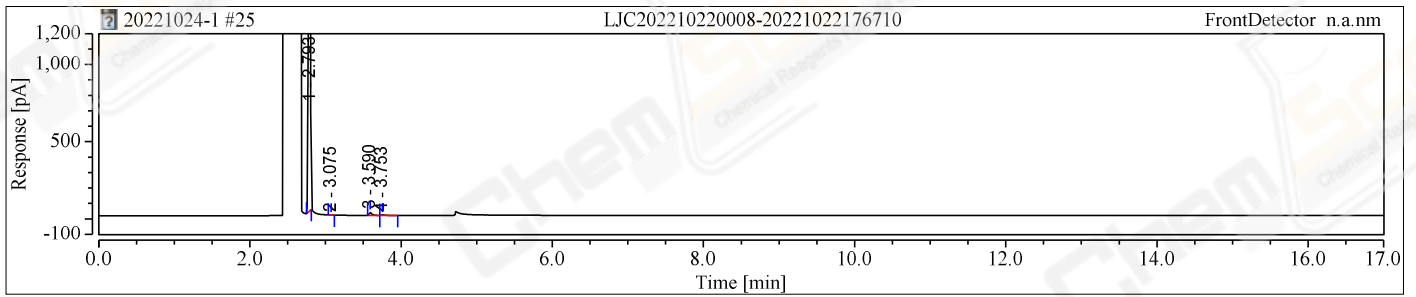


Chromatogram and Results

CAS NO.:	16545-68-9	Comment:	AH-GC003
Batch No:		Channel:	FrontDetector
Vial Number:	24	Wavelength:	n.a.
Injection Type:	Unknown	Injection Volume:	1.00
Instrument:	GC10402	Injection Time:	24/10/2022 18:17
Instrument Method:	GC-FQ	InstMeth.creation_t	11/05/2020 11:09
Processing Method:	PM-LJC202210220008-20221022176710	Last update_time:	25/10/2022 09:29
seq.creation_operator	Myangby		
chrom://ahyy-cm7/CM7DATA/Leyan/GC10402/Sequence/2022/202210/20221024-1.seq/940.smp/FrontDetector.channel/FrontDetector.chm			

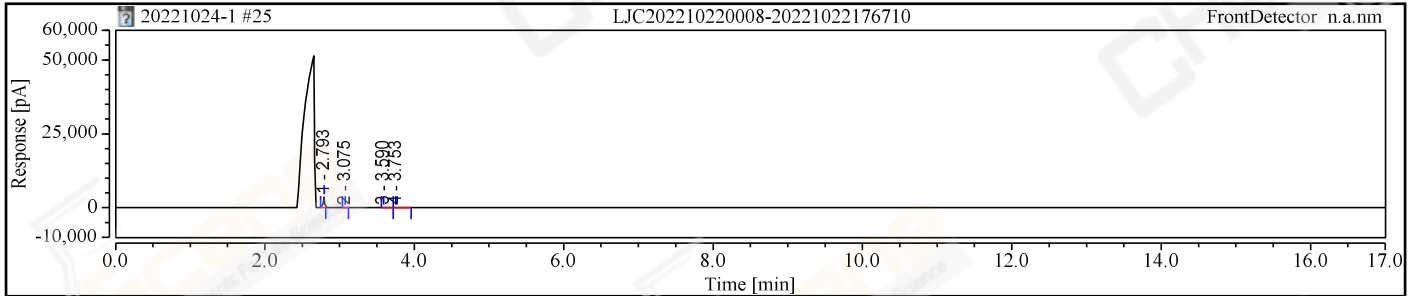

No.	Retention Time min	Area pA*min	Height pA	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	2.793	78.700	3610.909	110776	5.92	0.68	98.595	
2	3.075	0.007	0.131	39857	8.01	1.03	0.008	
3	3.590	0.900	19.867	46007	2.05	1.89	1.128	
4	3.753	0.215	3.138	26582	n.a.	2.94	0.269	
Total:		79.822	3634.044		15.98			