
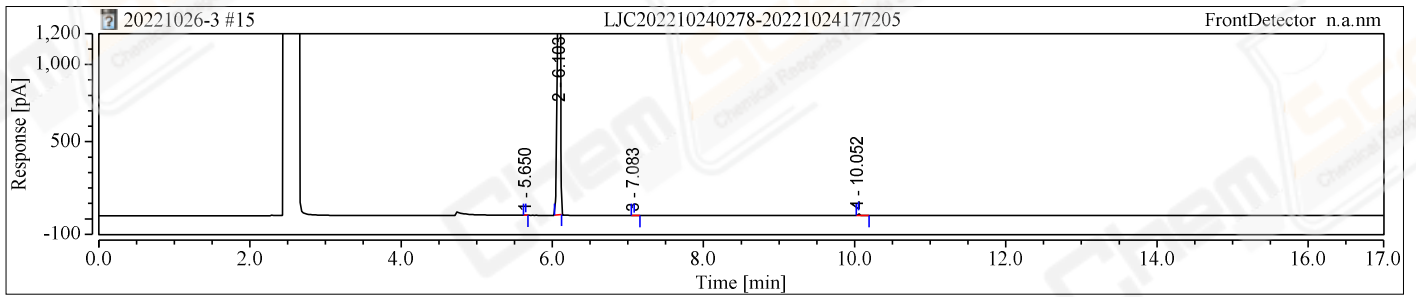


Chromatogram and Results

CAS NO.:	1011460-68-6	Comment:	AH-GC003
Batch No:	1157099	Channel:	FrontDetector
Vial Number:	14	Wavelength:	n.a.
Injection Type:	Unknown	Injection Volume:	1.00
Instrument:	GC10402	Injection Time:	26/10/2022 21:31
Instrument Method:	GC-FQ	InstMeth.creation_t	11/05/2020 11:09
Processing Method:	PM-LJC202210240278-20221024177205	Last update_time:	27/10/2022 09:08
seq.creation_operator	Lihui		
chrom://ahyy-cm7/CM7DATA/Leyan/GC10402/Sequence/2022/202210/20221026-3.seq/596.smp/FrontDetector.channel/FrontDetector.chm			

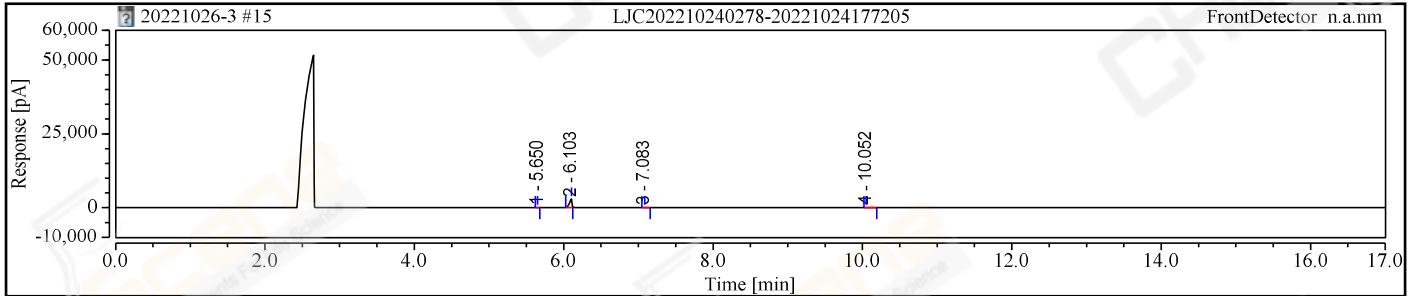

No.	Retention Time min	Area pA*min	Height pA	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	5.650	0.009	0.349	347916	8.71	0.99	0.008	
2	6.103	108.560	2932.147	137803	17.77	0.62	99.633	
3	7.083	0.018	0.575	404343	72.09	1.88	0.016	
4	10.052	0.373	13.985	1131882	n.a.	1.56	0.342	
Total:		108.960	2947.056		98.57			