
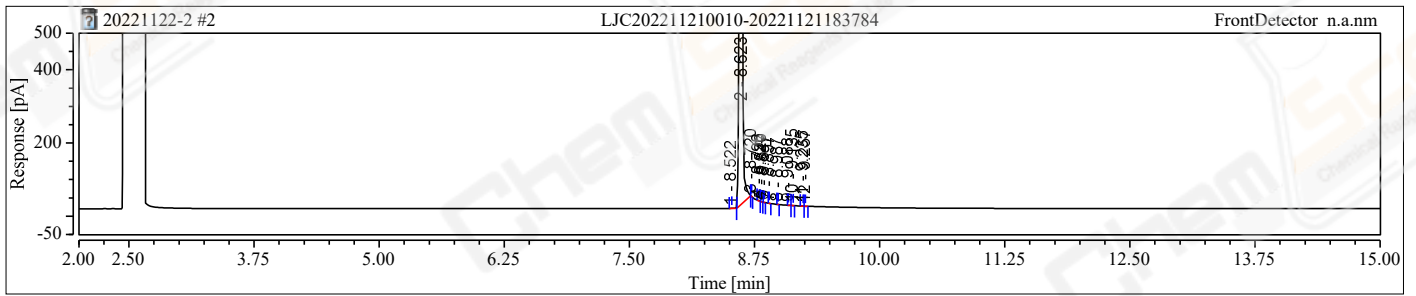


Chromatogram and Results

CAS NO.:	104-54-1	Comment:	AH-GC003
Batch No:	1015585	Channel:	FrontDetector
Vial Number:	43	Wavelength:	n.a.
Injection Type:	Unknown	Injection Volume:	1.00
Instrument:	GC10402	Injection Time:	22/11/2022 15:30
Instrument Method:	GC-FQ	InstMeth.creation_t	11/05/2020 11:09
Processing Method:	PM-LJC202211210010-20221121183784	Last update_time:	23/11/2022 10:50
seq.creation_operator	Myuxp		
chrom://ahyy-cm7/CM7DATA/Leyan/GC10402/Sequence/2022/202211/20221122-2.seq/339.smp/FrontDetector.channel/FrontDetector.chm			

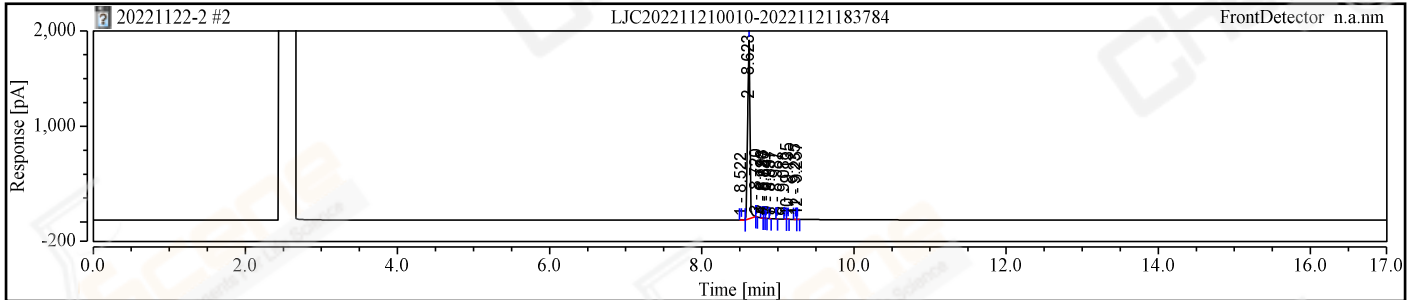

No.	Retention Time min	Area pA*min	Height pA	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	8.522	0.043	1.186	329539	1.80	1.54	0.073	
2	8.623	59.069	1869.296	418805	2.86	0.69	99.864	
3	8.720	0.004	0.522	5974820	2.21	1.13	0.008	
4	8.798	0.007	0.420	386468	0.36	0.71	0.012	
5	8.820	0.004	0.347	293604	0.55	1.09	0.007	
6	8.847	0.003	0.264	1243205	1.60	0.98	0.005	
7	8.897	0.005	0.336	1348977	2.50	1.21	0.008	
8	8.987	0.003	0.202	753458	2.85	0.90	0.004	
9	9.088	0.003	0.155	1463312	1.41	1.74	0.006	
10	9.135	0.003	0.183	1024075	2.29	0.80	0.005	
11	9.235	0.003	0.167	522636	0.36	0.70	0.006	
12	9.257	0.002	0.100	298167	n.a.	2.06	0.004	
Total:		59.150	1873.178		18.80			