
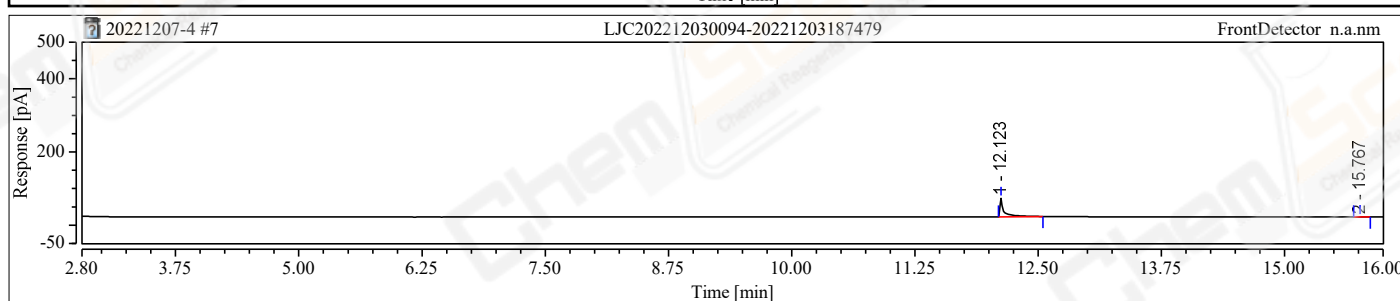


Chromatogram and Results

CAS NO.:	542-44-9	Comment:	AH-GC003
Batch No:		Channel:	FrontDetector
Vial Number:	34	Wavelength:	n.a.
Injection Type:	Unknown	Injection Volume:	1.00
Instrument:	GC10402	Injection Time:	07/12/2022 18:29
Instrument Method:	GC-FQ	InstMeth.creation_t	11/05/2020 11:09
Processing Method:	PM-LJC202212030094-20221203187479	Last update_time:	08/12/2022 09:22
seq.creation_operator	Myuxp		
chrom://ahyy-cm7/CM7DATA/Leyan/GC10402/Sequence/2022/202212/20221207-4.seq/630.smp/FrontDetector.channel/FrontDetector.chm			

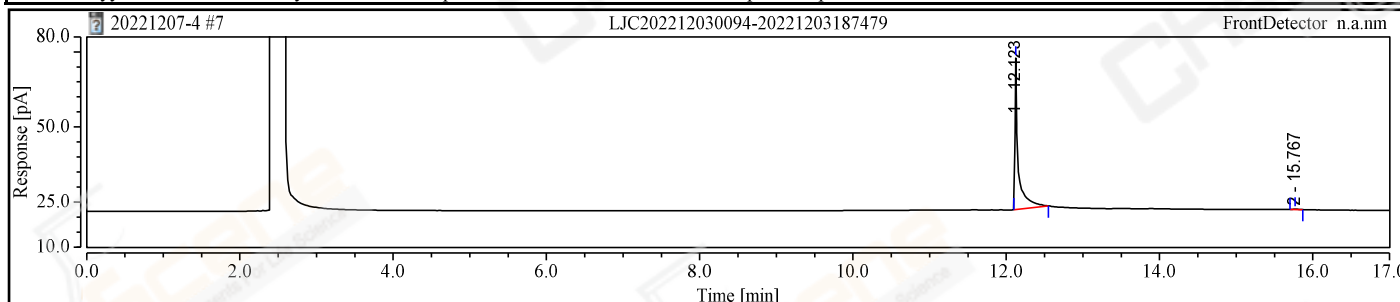

No.	Retention Time min	Area pA*min	Height pA	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	12.123	2.464	50.407	1481280	40.48	5.26	99.422	
2	15.767	0.014	0.185	202483	n.a.	1.31	0.578	
Total:		2.479	50.592		40.48			