
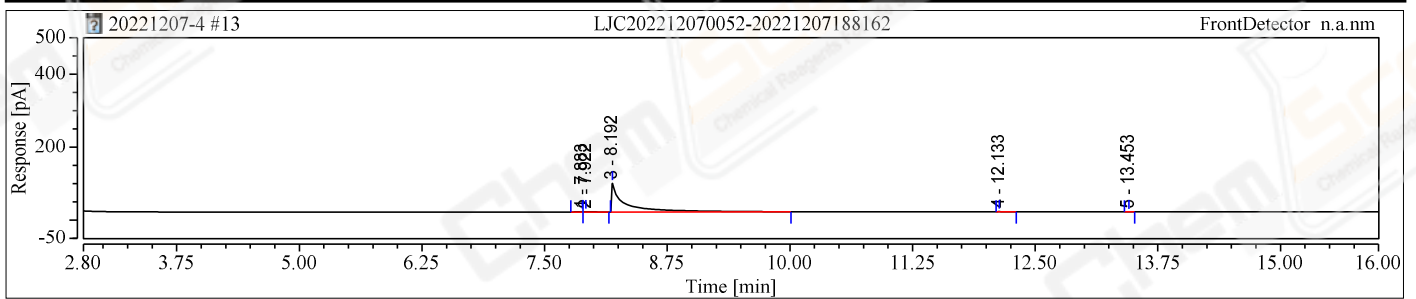


Chromatogram and Results

CAS NO.:	35344-95-7	Comment:	AH-GC003
Batch No:		Channel:	FrontDetector
Vial Number:	40	Wavelength:	n.a.
Injection Type:	Unknown	Injection Volume:	1.00
Instrument:	GC10402	Injection Time:	07/12/2022 20:41
Instrument Method:	GC-FQ	InstMeth.creation_t	11/05/2020 11:09
Processing Method:	PM-LJC202212070052-20221207188162	Last update_time:	08/12/2022 09:22
seq.creation_operator	Myuxp		
chrom://ahyy-cm7/CM7DATA/Leyan/GC10402/Sequence/2022/202212/20221207-4.seq/538.smp/FrontDetector.channel/FrontDetector.chm			

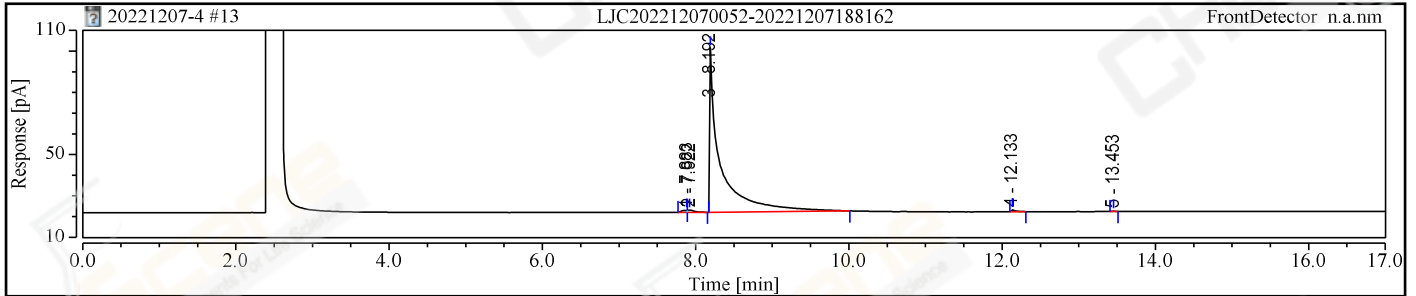

No.	Retention Time min	Area pA*min	Height pA	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	7.883	0.088	1.050	395	0.03	n.a.	0.681	
2	7.922	0.120	1.129	1868	0.66	n.a.	0.929	
3	8.192	12.693	79.407	151696	50.36	21.64	97.870	
4	12.133	0.061	0.991	449206	21.41	3.44	0.467	
5	13.453	0.007	0.181	1117220	n.a.	1.18	0.053	
Total:		12.969	82.758		72.46			