
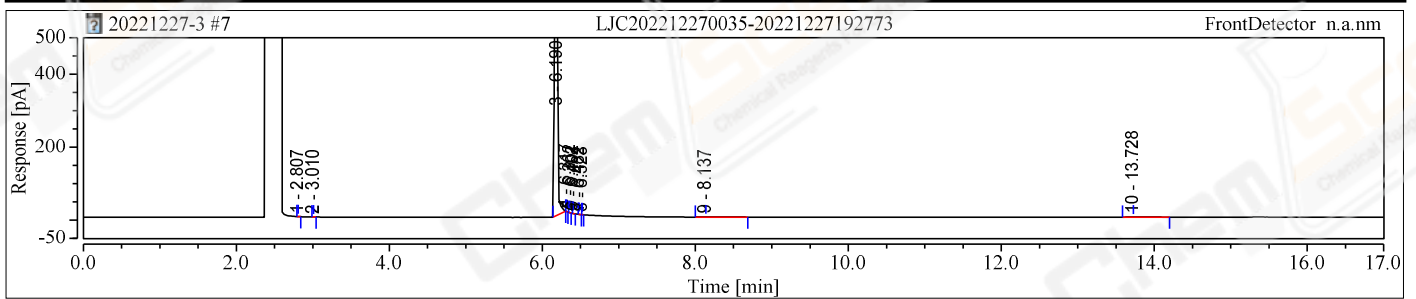


## Chromatogram and Results

CAS NO.:	944401-77-8	Comment:	AH-GC003
Batch No:	1062631	Channel:	FrontDetector
Vial Number:	40	Wavelength:	n.a.
Injection Type:	Unknown	Injection Volume:	1.00
Instrument:	GC10402	Injection Time:	28/12/2022 00:35
Instrument Method:	GC-FQ	InstMeth.creation_t	11/05/2020 11:09
Processing Method:	PM-LJC202212270035-20221227192773	Last update_time:	28/12/2022 10:48
seq.creation_operator	Myangby		
chrom://ahyy-cm7/CM7DATA/Leyan/GC10402/Sequence/2022/202212/20221227-3.seq/986.smp/FrontDetector.channel/FrontDetector.chm			

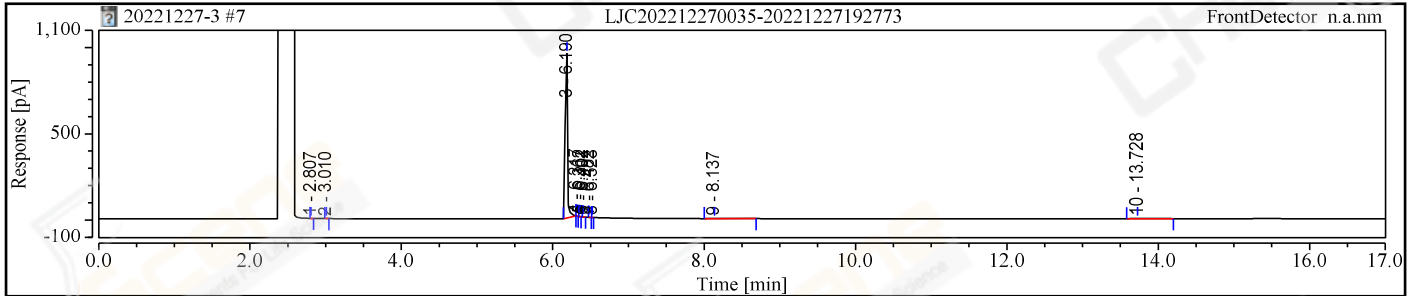

No.	Retention Time min	Area pA*min	Height pA	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	2.807	0.004	0.152	97332	5.42	1.66	0.009	
2	3.010	0.004	0.178	95378	64.09	1.30	0.012	
3	6.190	37.869	951.817	168912	2.17	0.75	98.295	
4	6.317	0.006	0.322	200476	1.15	1.29	0.015	
5	6.362	0.006	0.466	1339374	1.70	0.87	0.017	
6	6.402	0.008	0.382	1033980	3.51	2.38	0.021	
7	6.482	0.004	0.197	1624291	2.05	1.99	0.009	
8	6.523	0.003	0.218	1652595	3.58	1.43	0.008	
9	8.137	0.339	0.931	1364	7.97	2.55	0.880	
10	13.728	0.284	0.871	11039	n.a.	2.19	0.736	
Total:		38.526	955.534		91.64			