
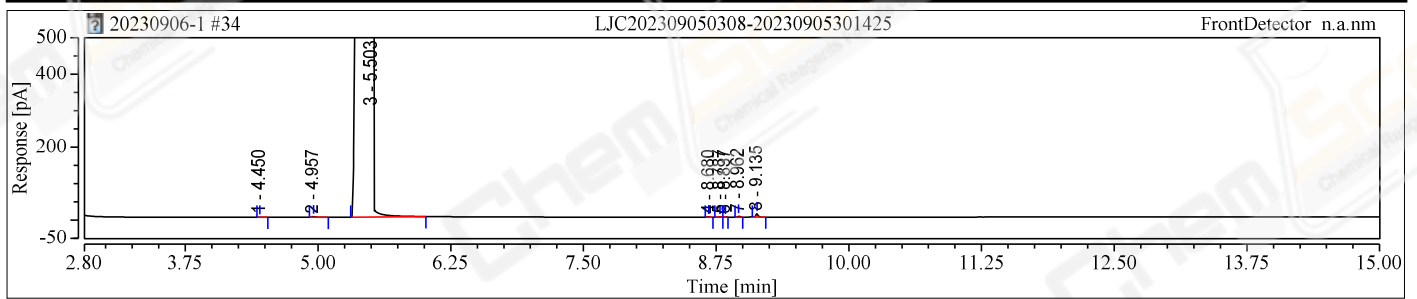


Chromatogram and Results

CAS NO.:	108-93-0	Comment:	AH-GC039
Batch No:		Channel:	FrontDetector
Vial Number:	34	Wavelength:	n.a.
Injection Type:	Unknown	Injection Volume:	1.00
Instrument:	GC10402	Injection Time:	06/09/2023 22:09
Instrument Method:	GC-FQ	InstMeth.creation_t	11/05/2020 11:09
Processing Method:	LJC202309050308-20230905301425	Last update_time:	07/09/2023 10:23
seq.creation_operator	Yuxiaoping		
chrom://ahyy-cm7/CM7DATA/Leyan/GC10402/Sequence/2023/202309/20230906-1.seq/482.smp/FrontDetector.channel/FrontDetector.chm			

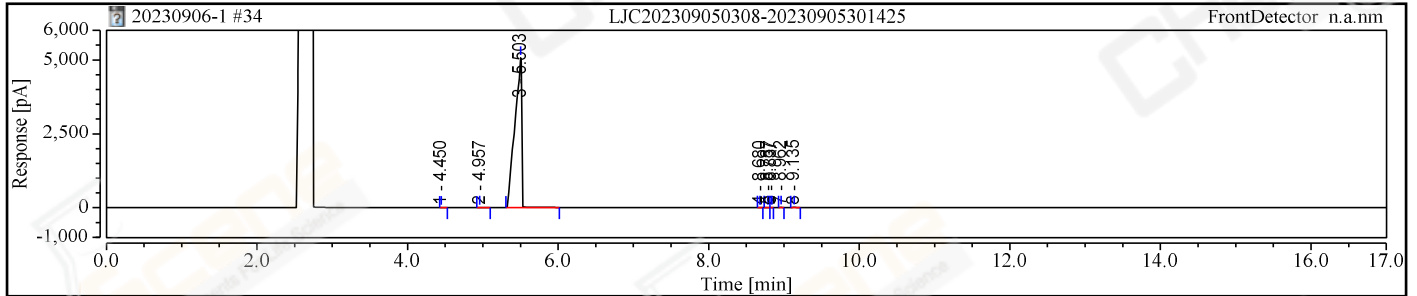

No.	Retention Time min	Area pA*min	Height pA	Plates (EP)	Resolution (EP)	Asymmetry (EP)	Rel.Area %	Peak Name
1	4.450	0.012	0.314	107077	7.94	2.00	0.002	
2	4.957	0.084	1.683	72787	4.50	2.04	0.016	
3	5.503	513.815	5060.493	16772	30.77	0.56	99.923	
4	8.680	0.015	0.652	877566	2.94	1.10	0.003	
5	8.787	0.010	0.416	970065	1.43	0.77	0.002	
6	8.837	0.012	0.586	1060454	3.61	1.01	0.002	
7	8.962	0.060	2.706	1047378	5.00	1.14	0.012	
8	9.135	0.200	9.085	1123318	n.a.	1.02	0.039	
Total:		514.210	5075.934		56.20			