
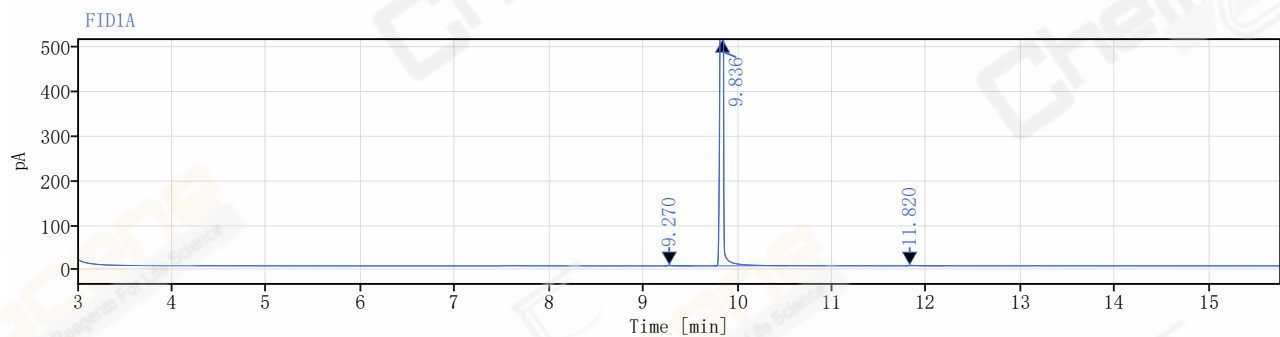


# Chromatogram and Results

<b>CAS NO. :</b>	627871-16-3	<b>Instrument:</b>	8860
<b>Batch No:</b>		<b>Sequence Name:</b>	20231101-3
<b>seq.creation operator:</b>	yuxiaoping	<b>Injection:</b>	1.000 µL
<b>Vial Number:</b>	127	<b>Run Time:</b>	17
<b>Instrument Method:</b>	GC-FQ.amx	<b>Injection Time:</b>	2023-11-01 17:47:26+08:00
<b>Processing Method:</b>	*LJC202311010005.pmx	<b>Column Type:</b>	HP-5
<b>chrom:</b>	/Leyan/Results/20231101-3.rslt		

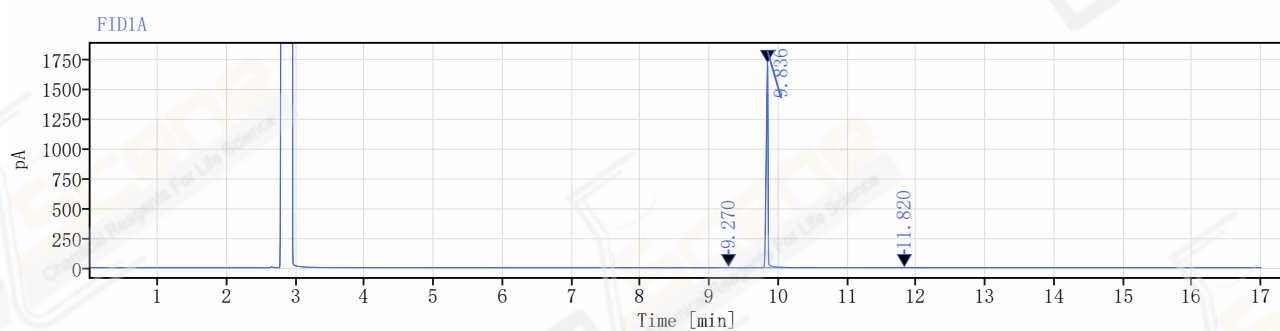

FID1A								
No.	RT [min]	Area	Height	Plates EP	Resolution EP	Asymmetry	Rel Area %	Peak Name
1	9.27	7.104	1.669	194147		4.35	0.222	
2	9.84	3185.469	1715.683	648479	8.53	0.67	99.480	
3	11.82	9.555	1.171	65195	16.99	5.88	0.298	
Total:		3202.13	1718.523		25.52		100.000	