


CAS NO.: 4506-66-5, D2O

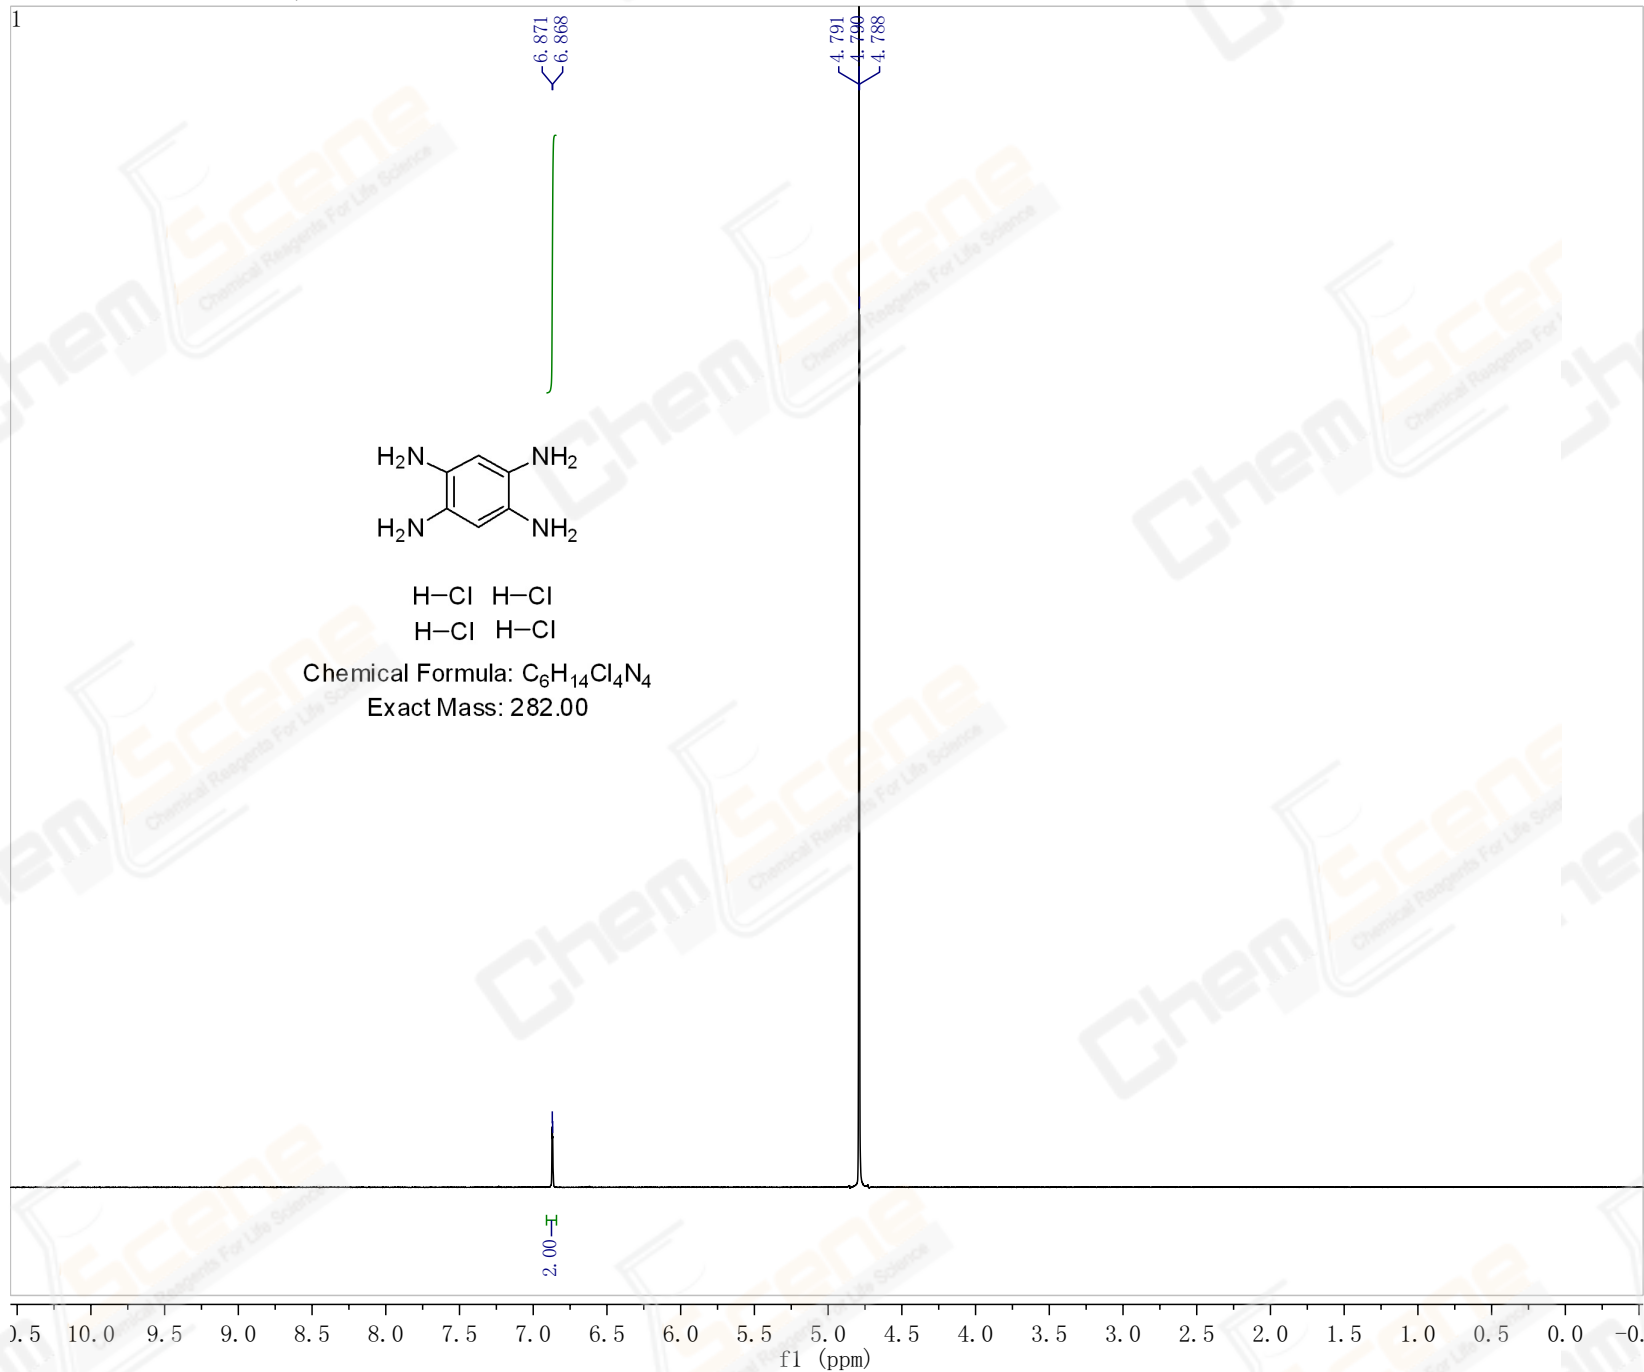

Parameters		
Parameter	Value	
1	Title	
2	Spectrometer	magnet
3	Solvent	D2O
4	Temperature	296.4
5	Pulse Sequence	s1pul30
6	Number of Scans	32
7	Receiver Gain	64
8	Relaxation Delay	1.0000
9	Pulse Width	9.8000
10	Acquisition Time	3.9999
11	Acquisition Date	2021-05-17T18:45:58
12	Modification Date	2021-05-17T18:57:48
13	Spectrometer Frequency	400.00
14	Spectral Width	8108.0
15	Lowest Frequency	-1654.0
16	Nucleus	$^1H$
17	Acquired Size	32431
18	Spectral Size	65536