


CAS NO.: 304456-62-0, DMSO

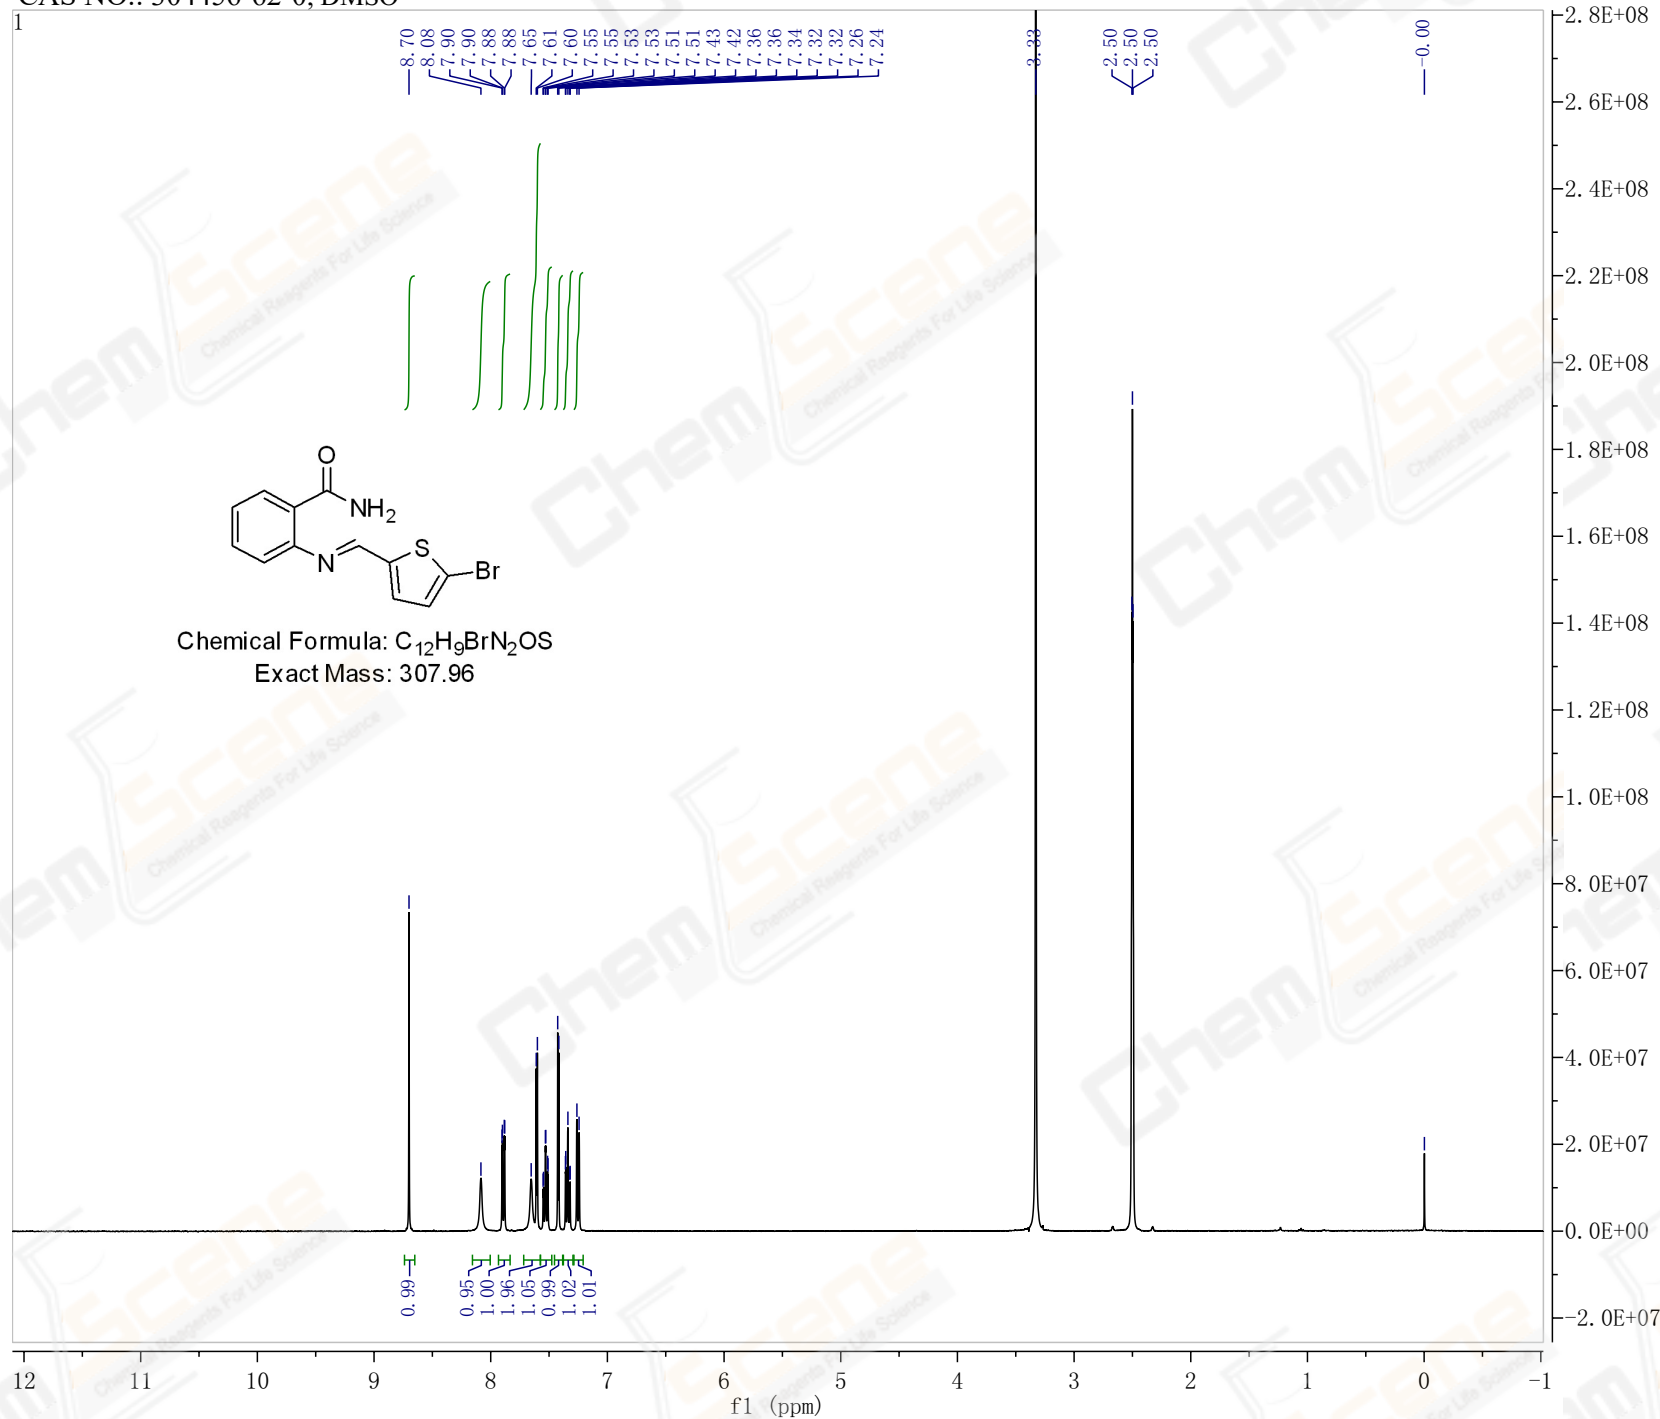

| Parameter                 | Value               |
|---------------------------|---------------------|
| 1 Title                   |                     |
| 2 Spectrometer magnet     |                     |
| 3 Solvent                 | DMSO                |
| 4 Temperature             | 296.8               |
| 5 Pulse Sequence          | slpul30             |
| 6 Number of Scans         | 64                  |
| 7 Receiver Gain           | 64                  |
| 8 Relaxation Delay        | 1.0000              |
| 9 Pulse Width             | 9.8000              |
| 10 Acquisition Time       | 3.9999              |
| 11 Acquisition Date       | 2021-06-03T20:24:03 |
| 12 Modification Date      | 2021-06-03T20:42:01 |
| 13 Spectrometer Frequency | 400.00              |
| 14 Spectral Width         | 8108.0              |
| 15 Lowest Frequency       | -1654.0             |
| 16 Nucleus                | $^1H$               |
| 17 Acquired Size          | 32431               |
| 18 Spectral Size          | 65536               |