


CAS NO.: 1351761-44-8, CDC13

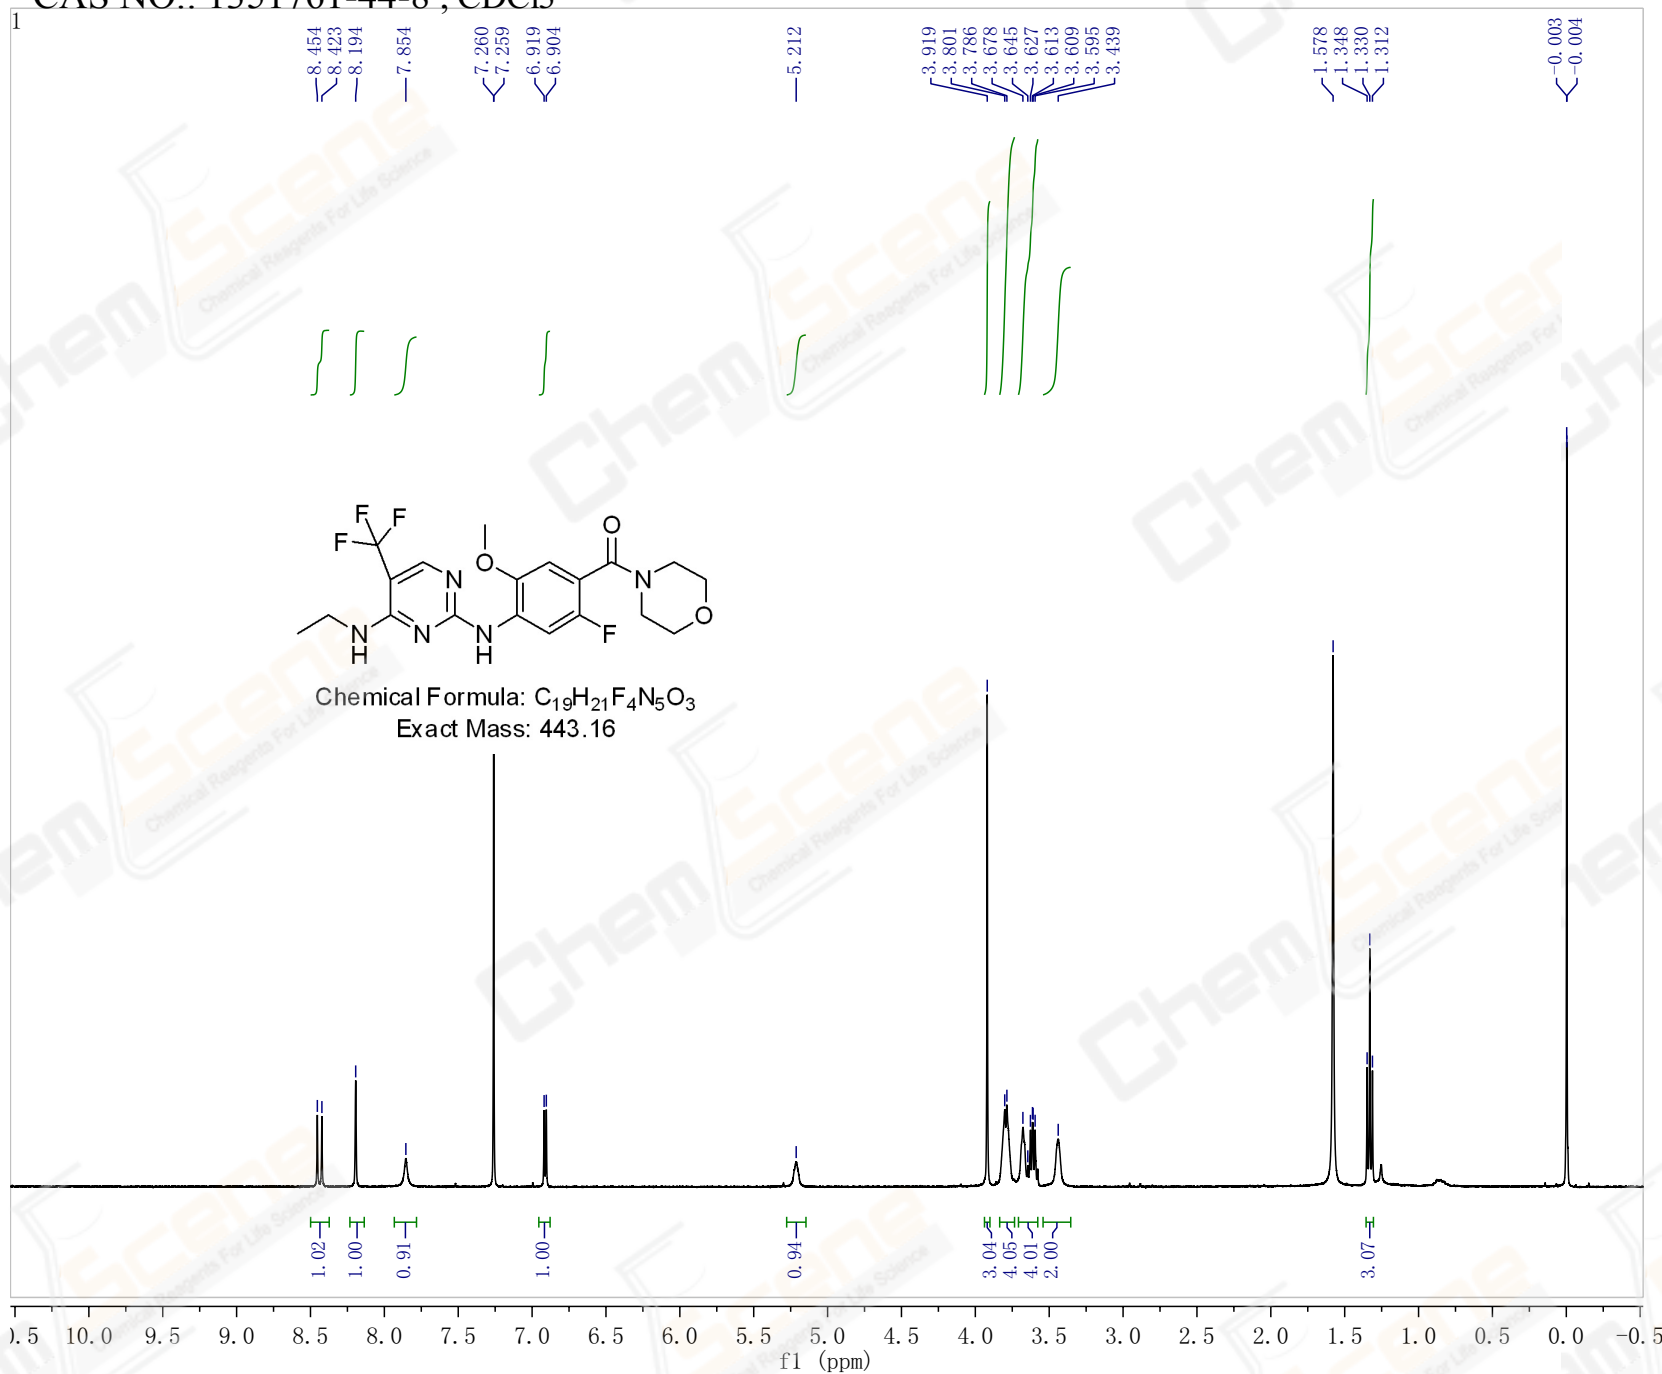

| Parameters |                        |                     |
|------------|------------------------|---------------------|
| Parameter  | Value                  |                     |
| 1          | Title                  |                     |
| 2          | Spectrometer           | magnet              |
| 3          | Solvent                | CDCl3               |
| 4          | Temperature            | 273.1               |
| 5          | Pulse Sequence         | s1pul30             |
| 6          | Number of Scans        | 64                  |
| 7          | Receiver Gain          | 64                  |
| 8          | Relaxation Delay       | 1.0000              |
| 9          | Pulse Width            | 9.8000              |
| 10         | Acquisition Time       | 3.9999              |
| 11         | Acquisition Date       | 2021-07-05T21:32:10 |
| 12         | Modification Date      | 2021-07-05T21:50:10 |
| 13         | Spectrometer Frequency | 400.00              |
| 14         | Spectral Width         | 8108.0              |
| 15         | Lowest Frequency       | -1654.0             |
| 16         | Nucleus                | $^1H$               |
| 17         | Acquired Size          | 32431               |
| 18         | Spectral Size          | 65536               |