


CAS NO.: 881375-00-4, CDCL3

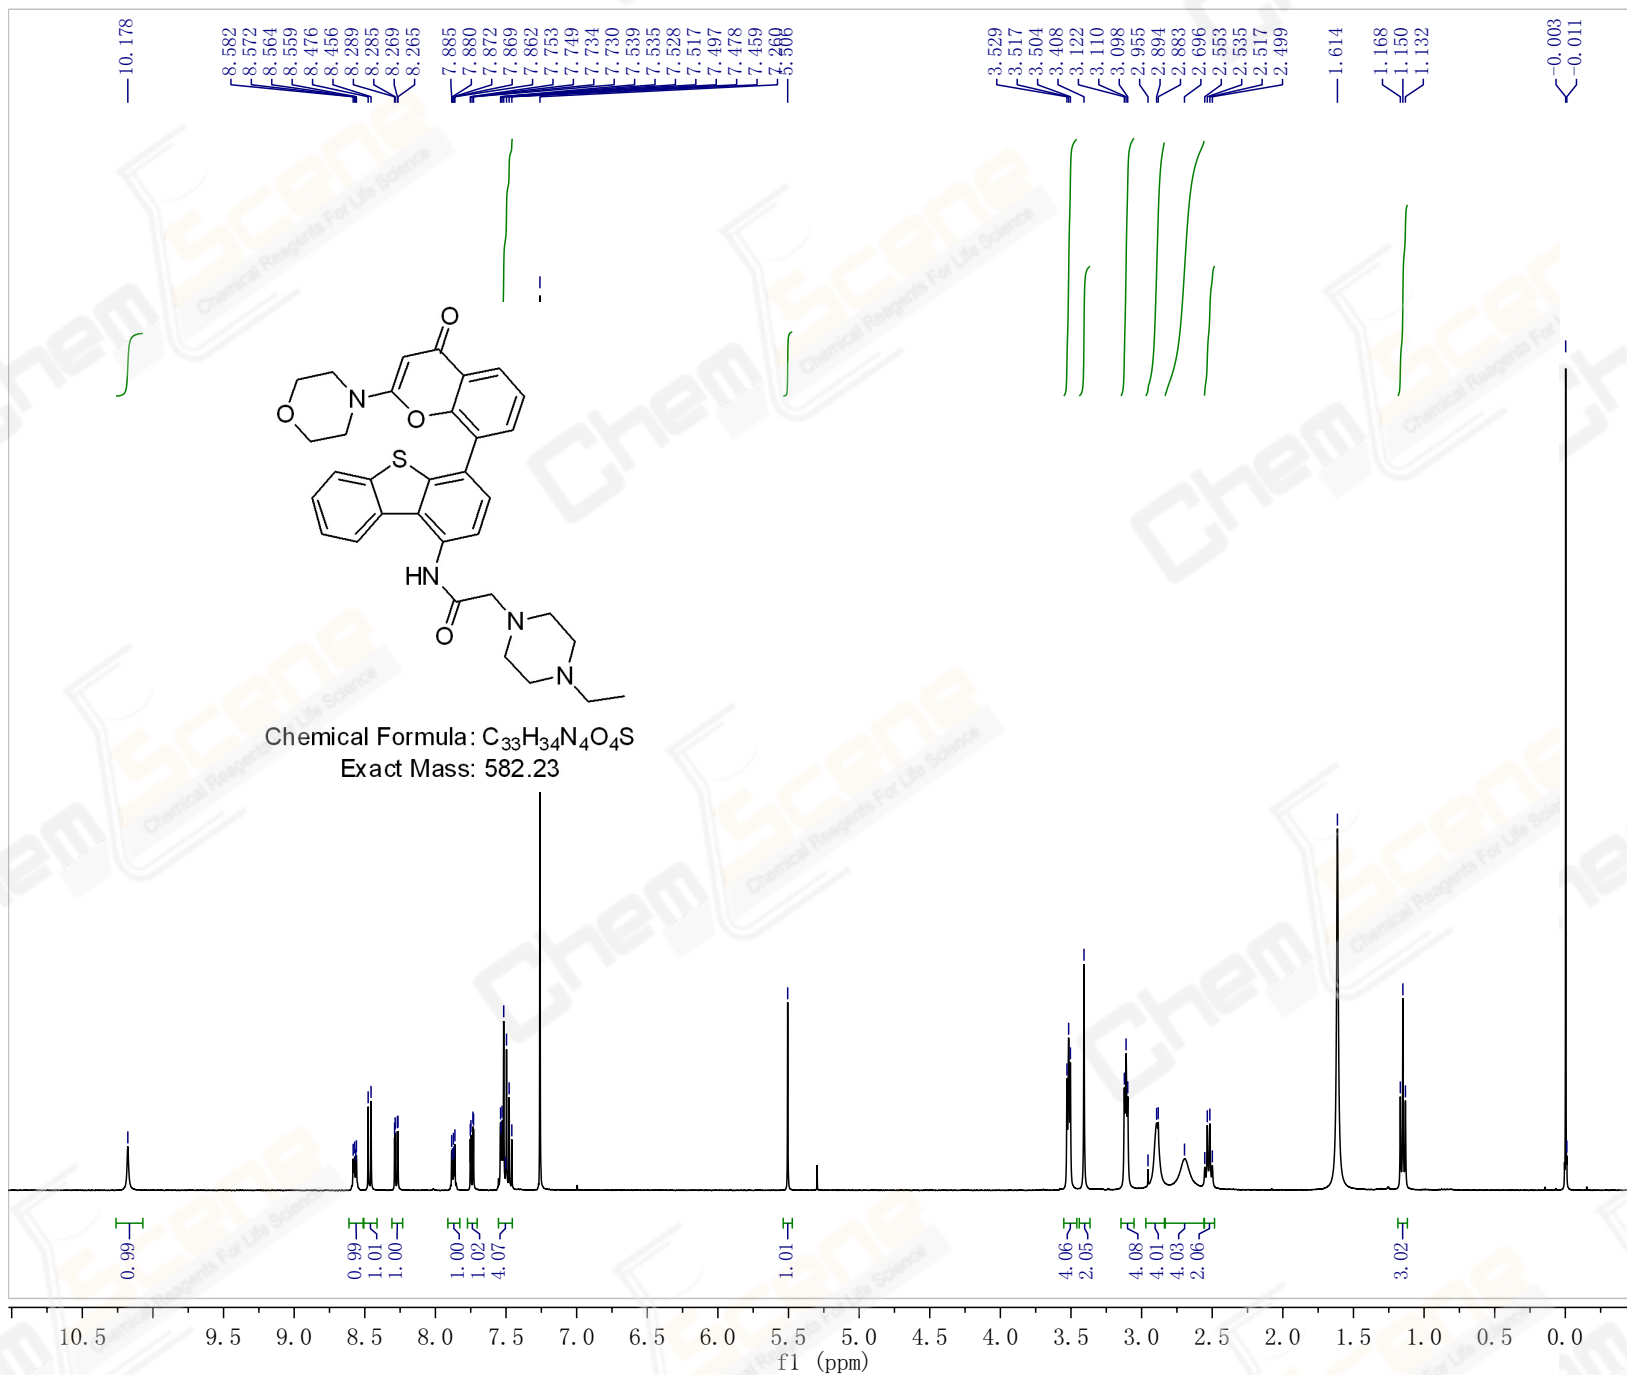

Parameters	
Parameter	Value
1	Title
2	Spectrometer
3	Solvent CDCl3
4	Temperature 298.0
5	Pulse Sequence zg30
6	Number of Scans 16
7	Receiver Gain 32
8	Relaxation Delay 1.0000
9	Pulse Width 10.0000
10	Acquisition Time 3.9977
11	Acquisition Date 1970-01-01T08:00:00
12	Modification Date 2021-09-01T12:33:56
13	Spectrometer Frequency 400.13
14	Spectral Width 8196.7
15	Lowest Frequency -5725.9
16	Nucleus 1H
17	Acquired Size 32768
18	Spectral Size 65536