


CAS NO.: 1702816-75-8, CDCL3

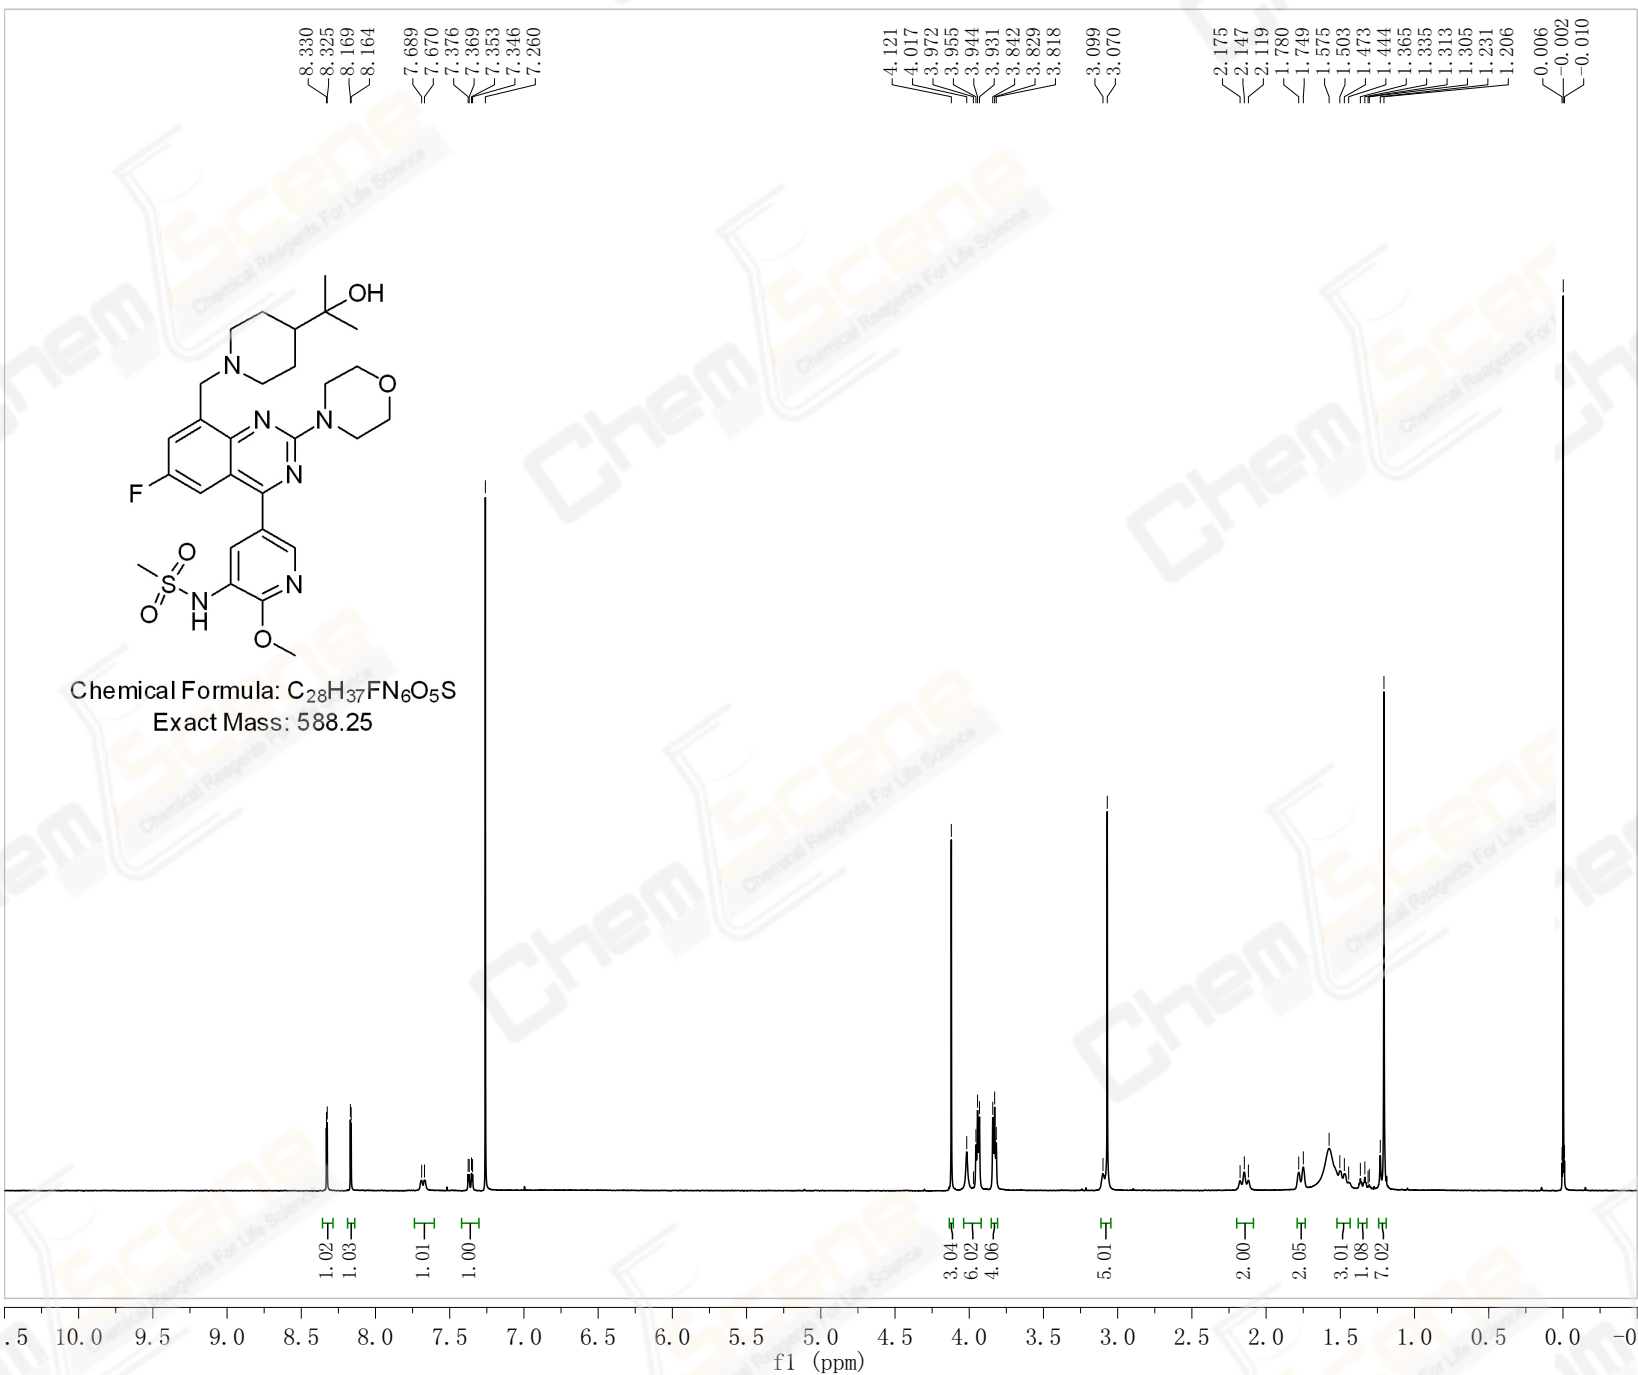

Parameter	Value
1 Title	
2 Spectrometer	
3 Solvent	
4 Temperature	298.0
5 Pulse Sequence	zg30
6 Number of Scans	16
7 Receiver Gain	32
8 Relaxation Delay	1.0000
9 Pulse Width	10.0000
10 Acquisition Time	3.9977
11 Acquisition Date	1970-01-01T08:00:00
12 Modification Date	2021-09-03T21:59:14
13 Spectrometer Frequency	400.13
14 Spectral Width	8196.7
15 Lowest Frequency	-5725.9
16 Nucleus	<sup>1</sup> H
17 Acquired Size	32768
18 Spectral Size	65536