


CAS NO.: 67-68-5, CDCL3

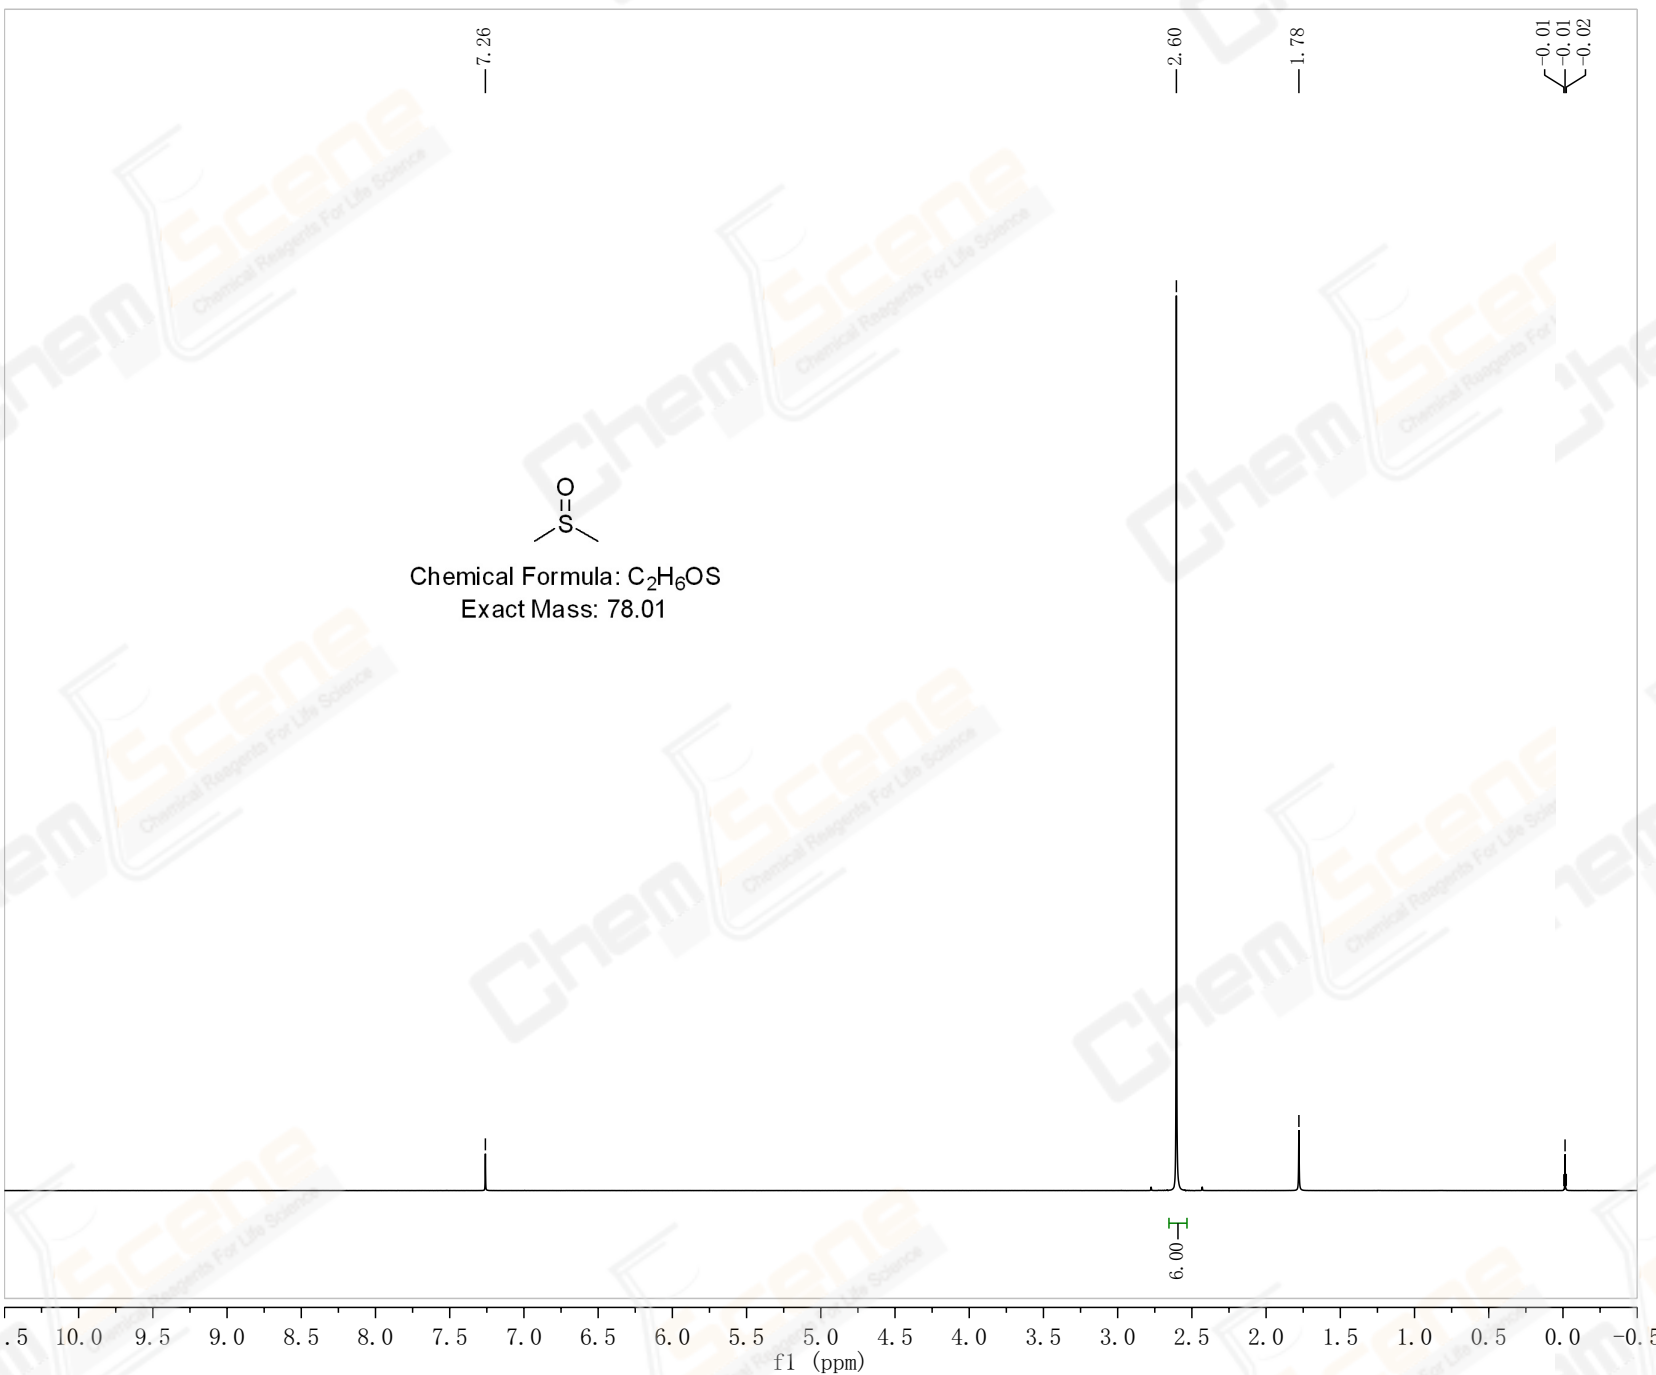

Parameter	Value
1 Title	
2 Spectrometer	magnet
3 Solvent	CDCl ₃
4 Temperature	298.1
5 Pulse Sequence	slpul30
6 Experiment	1D
7 Number of Scans	16
8 Receiver Gain	64
9 Relaxation Delay	1.0000
10 Pulse Width	9.8000
11 Acquisition Time	3.9999
12 Acquisition Date	2024-03-12T15:09:57
13 Modification Date	2024-03-12T15:19:31
14 Spectrometer Frequency	400.00
15 Spectral Width	8108.0
16 Lowest Frequency	-1654.0
17 Nucleus	¹ H
18 Acquired Size	32431
19 Spectral Size	65536