


CAS NO.: 327613-57-0, CDCL3

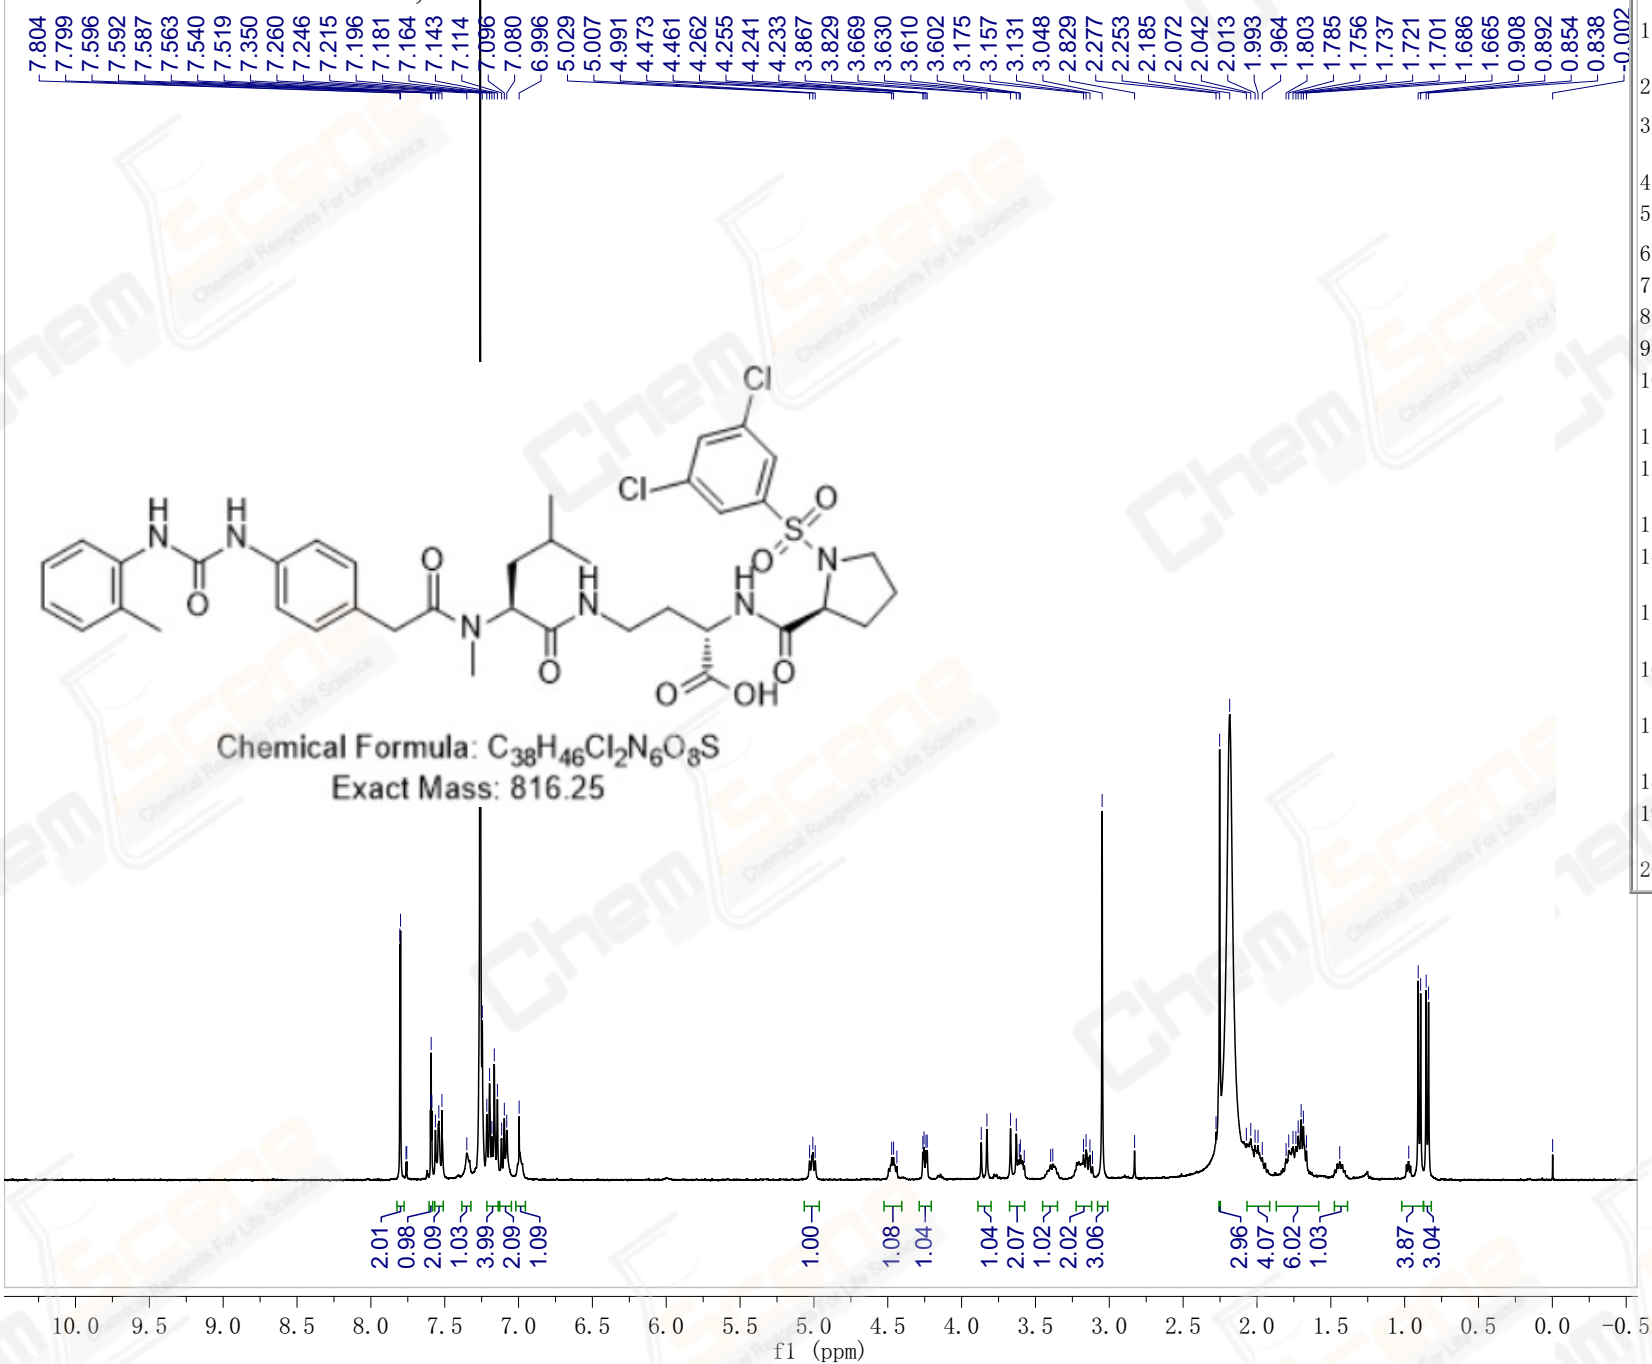

Parameter	Value
1 Title	SCH05
2 Comment	
3 Origin	Bruker BioSpin GmbH
4 Spectrometer	Avance
5 Author	
6 Solvent	CDCl3
7 Temperature	298.2
8 Pulse Sequence	zg30
9 Experiment	1D
10 Number of Scans	16
11 Receiver Gain	101
12 Relaxation Delay	1.0000
13 Pulse Width	8.0000
14 Acquisition Time	3.9977
15 Acquisition Date	2022-06-02T13:20:14
16 Modification Date	2022-06-02T13:23:28
17 Spectrometer Frequency	400.13
18 Spectral Width	8196.7
19 Lowest Frequency	-1636.5
20 Nucleus	1H