


CAS NO.: 106566-58-9, DMSO

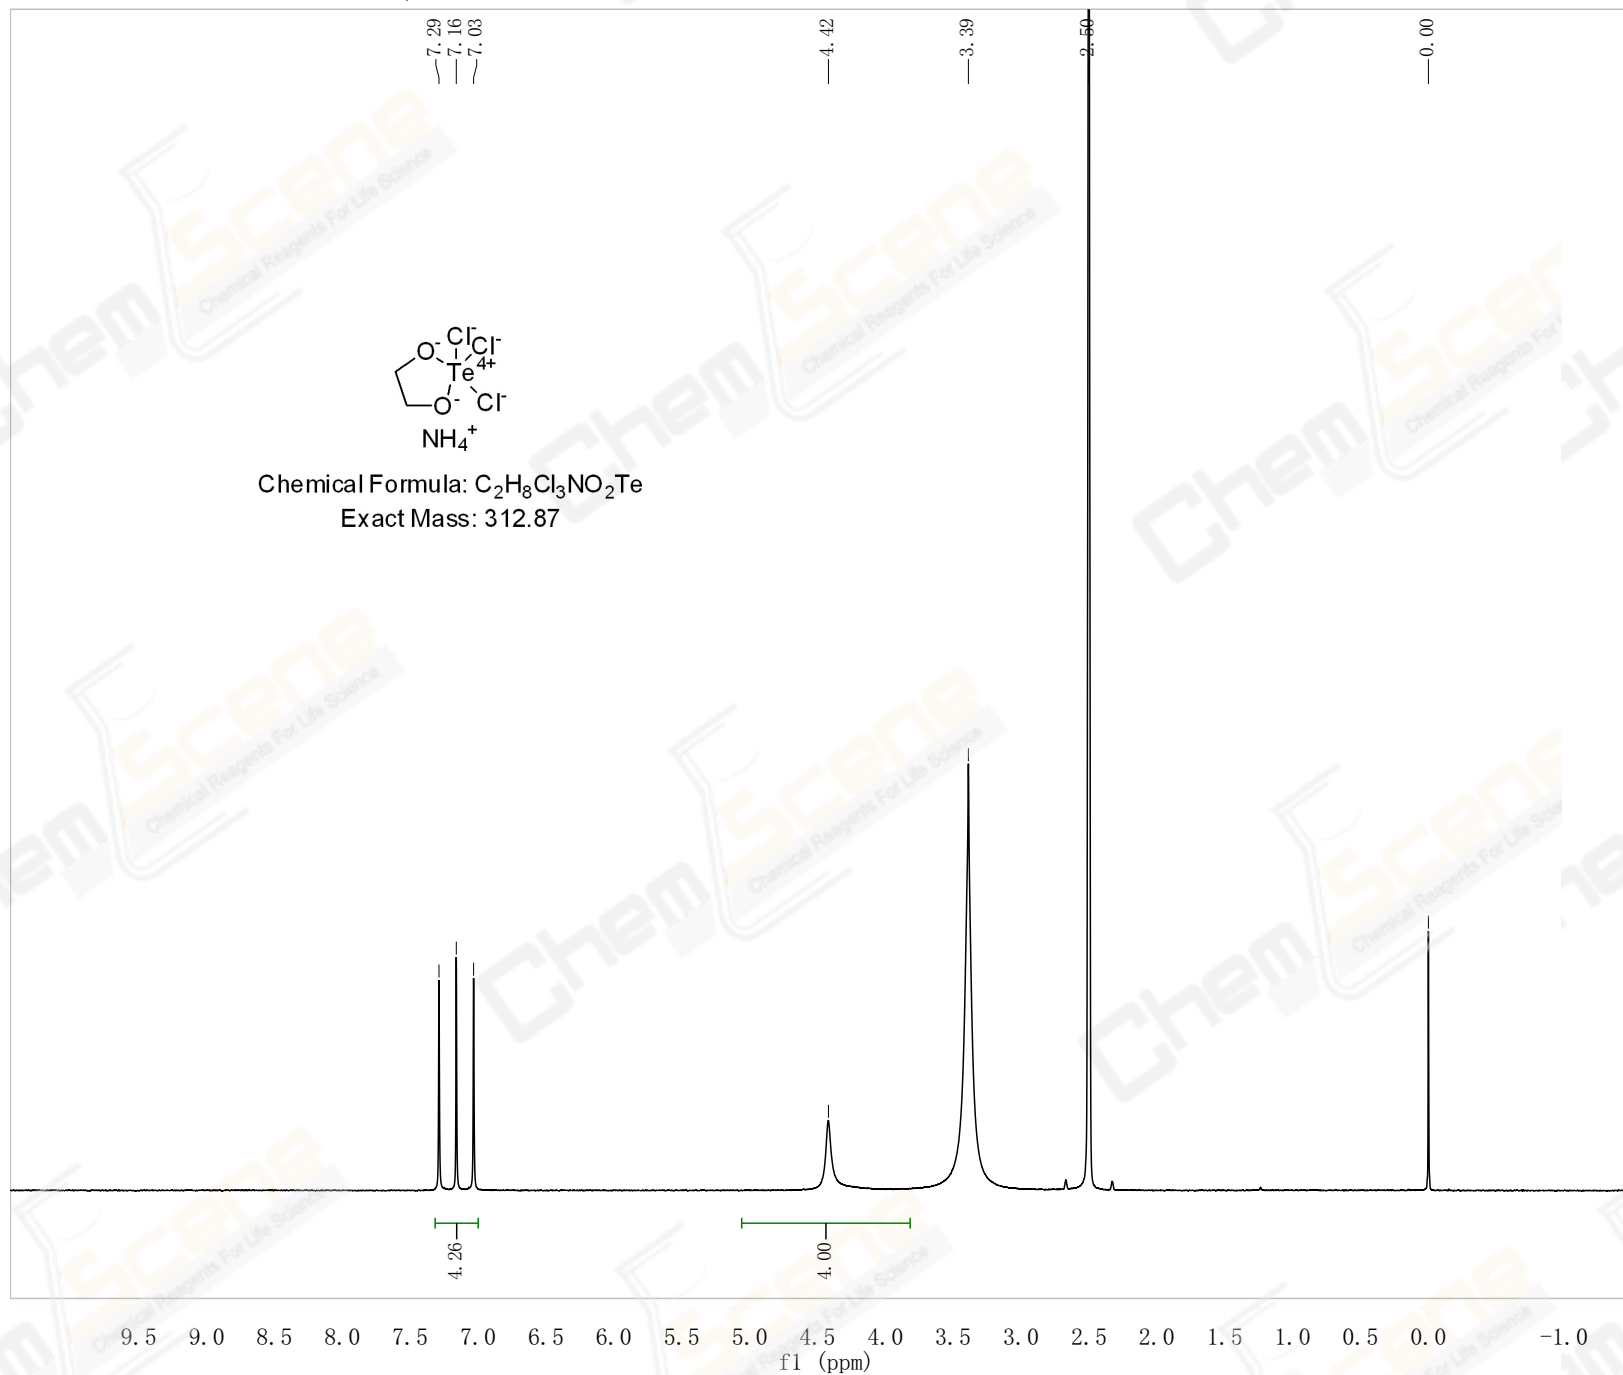

| Parameter | Value |
|---------------------------|---------------------|
| 1 Data File Name | // |
| 2 Title | BIZ2022-607-WLQ9 |
| 3 Comment | |
| 4 Origin | Bruker BioSpin GmbH |
| 5 Owner | nmrsu |
| 6 Site | |
| 7 Spectrometer | Avance |
| 8 Author | |
| 9 Solvent | DMSO |
| 10 Temperature | 298.2 |
| 11 Pulse Sequence | zg30 |
| 12 Experiment | 1D |
| 13 Number of Scans | 16 |
| 14 Receiver Gain | 101 |
| 15 Relaxation Delay | 1.0000 |
| 16 Pulse Width | 8.0000 |
| 17 Acquisition Time | 3.9977 |
| 18 Acquisition Date | 2022-06-10T07:49:12 |
| 19 Modification Date | 2022-06-10T07:52:27 |
| 20 Spectrometer Frequency | 400.13 |
| 21 Spectral Width | 8196.7 |
| 22 Lowest Frequency | -1630.6 |
| 23 Nucleus | 1H |
| 24 Acquired Size | 32768 |
| 25 Spectral Size | 65536 |