


CAS NO.: 1231930-82-7, CDCl₃

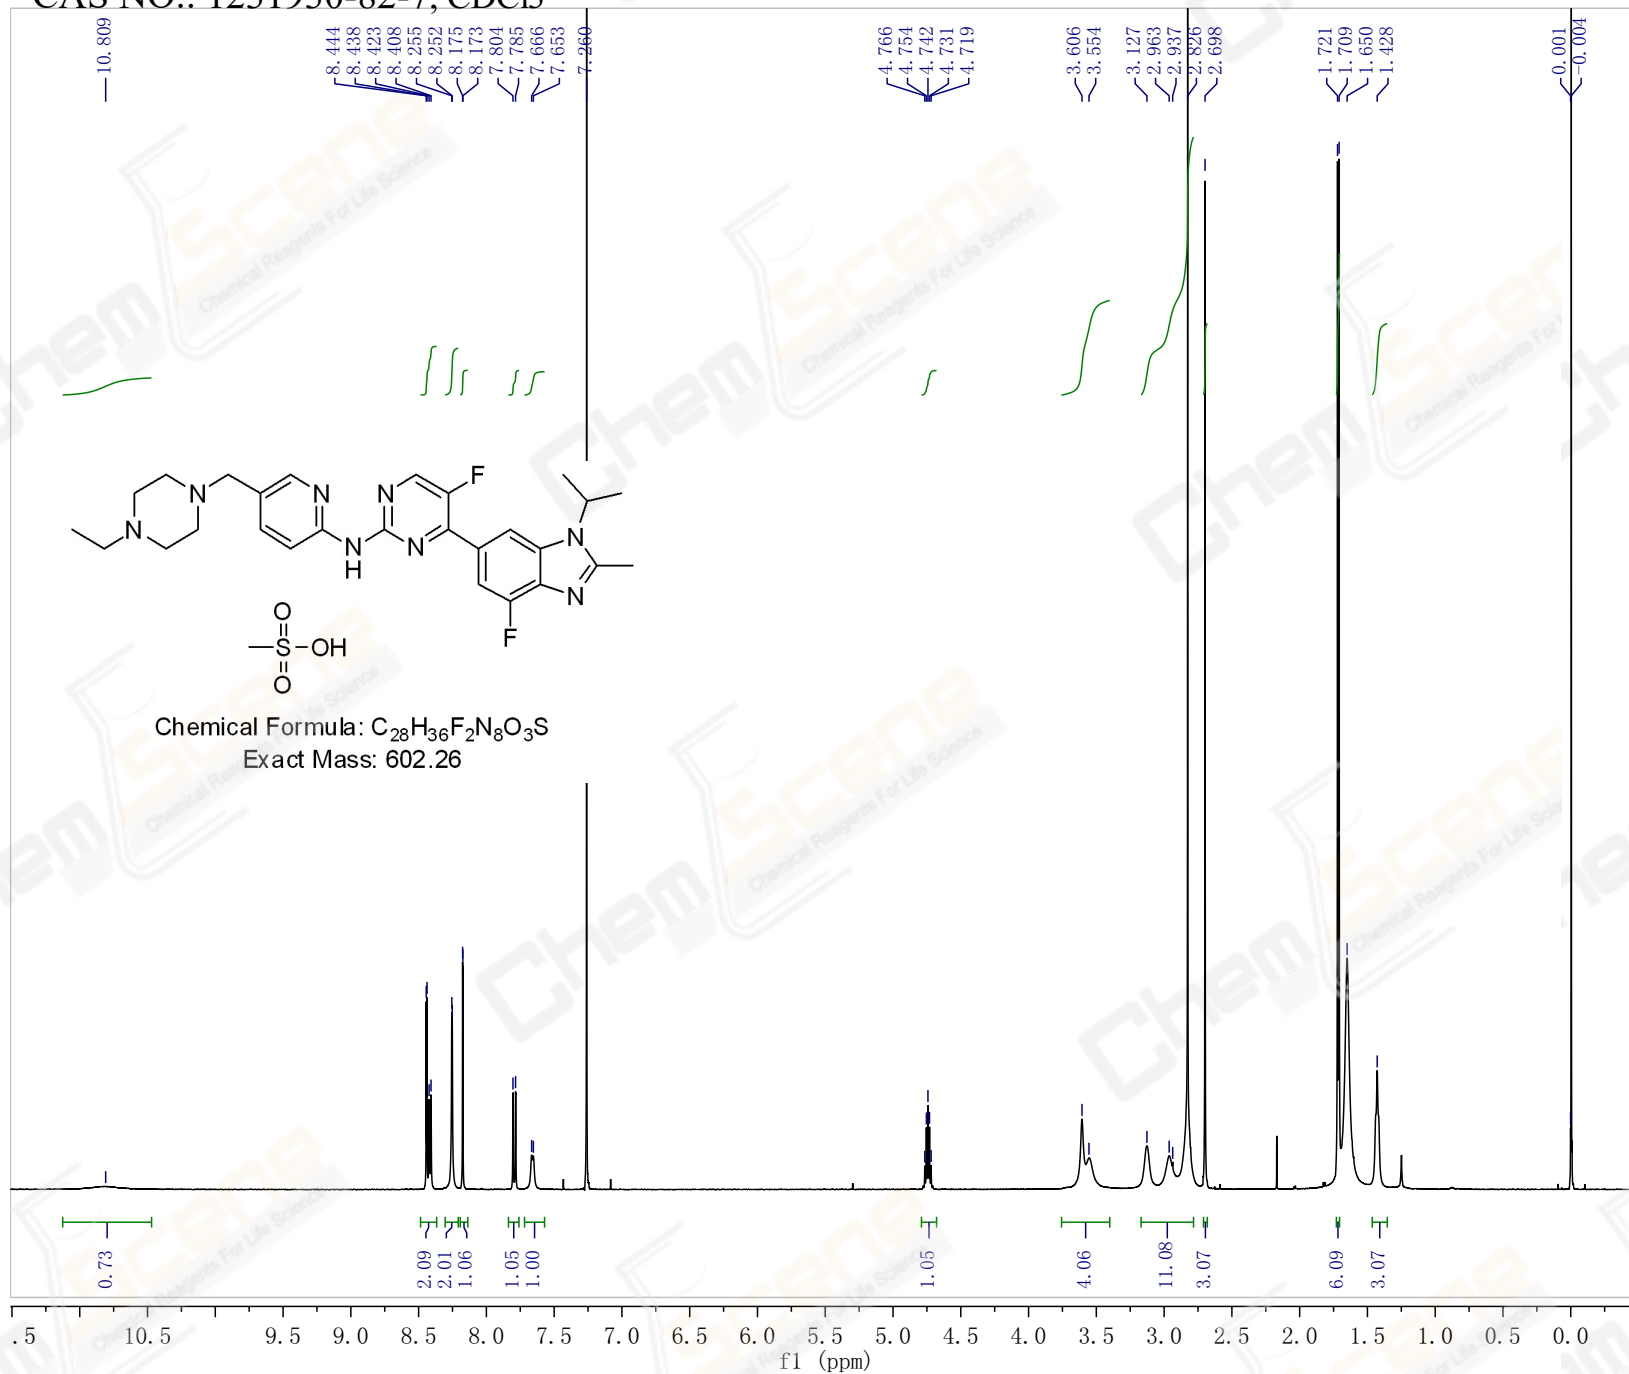

| Parameters | |
|---------------------------|---------------------|
| Parameter | Value |
| 1 Title | |
| 2 Spectrometer | spect |
| 3 Solvent | CDCl ₃ |
| 4 Temperature | 298.0 |
| 5 Pulse Sequence | zg30 |
| 6 Number of Scans | 16 |
| 7 Receiver Gain | 190 |
| 8 Relaxation Delay | 1.0000 |
| 9 Pulse Width | 10.0000 |
| 10 Acquisition Time | 2.7263 |
| 11 Acquisition Date | 2022-08-30T13:02:00 |
| 12 Modification Date | 2022-08-30T13:37:26 |
| 13 Spectrometer Frequency | 600.13 |
| 14 Spectral Width | 12019.2 |
| 15 Lowest Frequency | -2315.8 |
| 16 Nucleus | ¹ H |
| 17 Acquired Size | 32768 |
| 18 Spectral Size | 65536 |