


CAS NO.: 1115-70-4, D2O

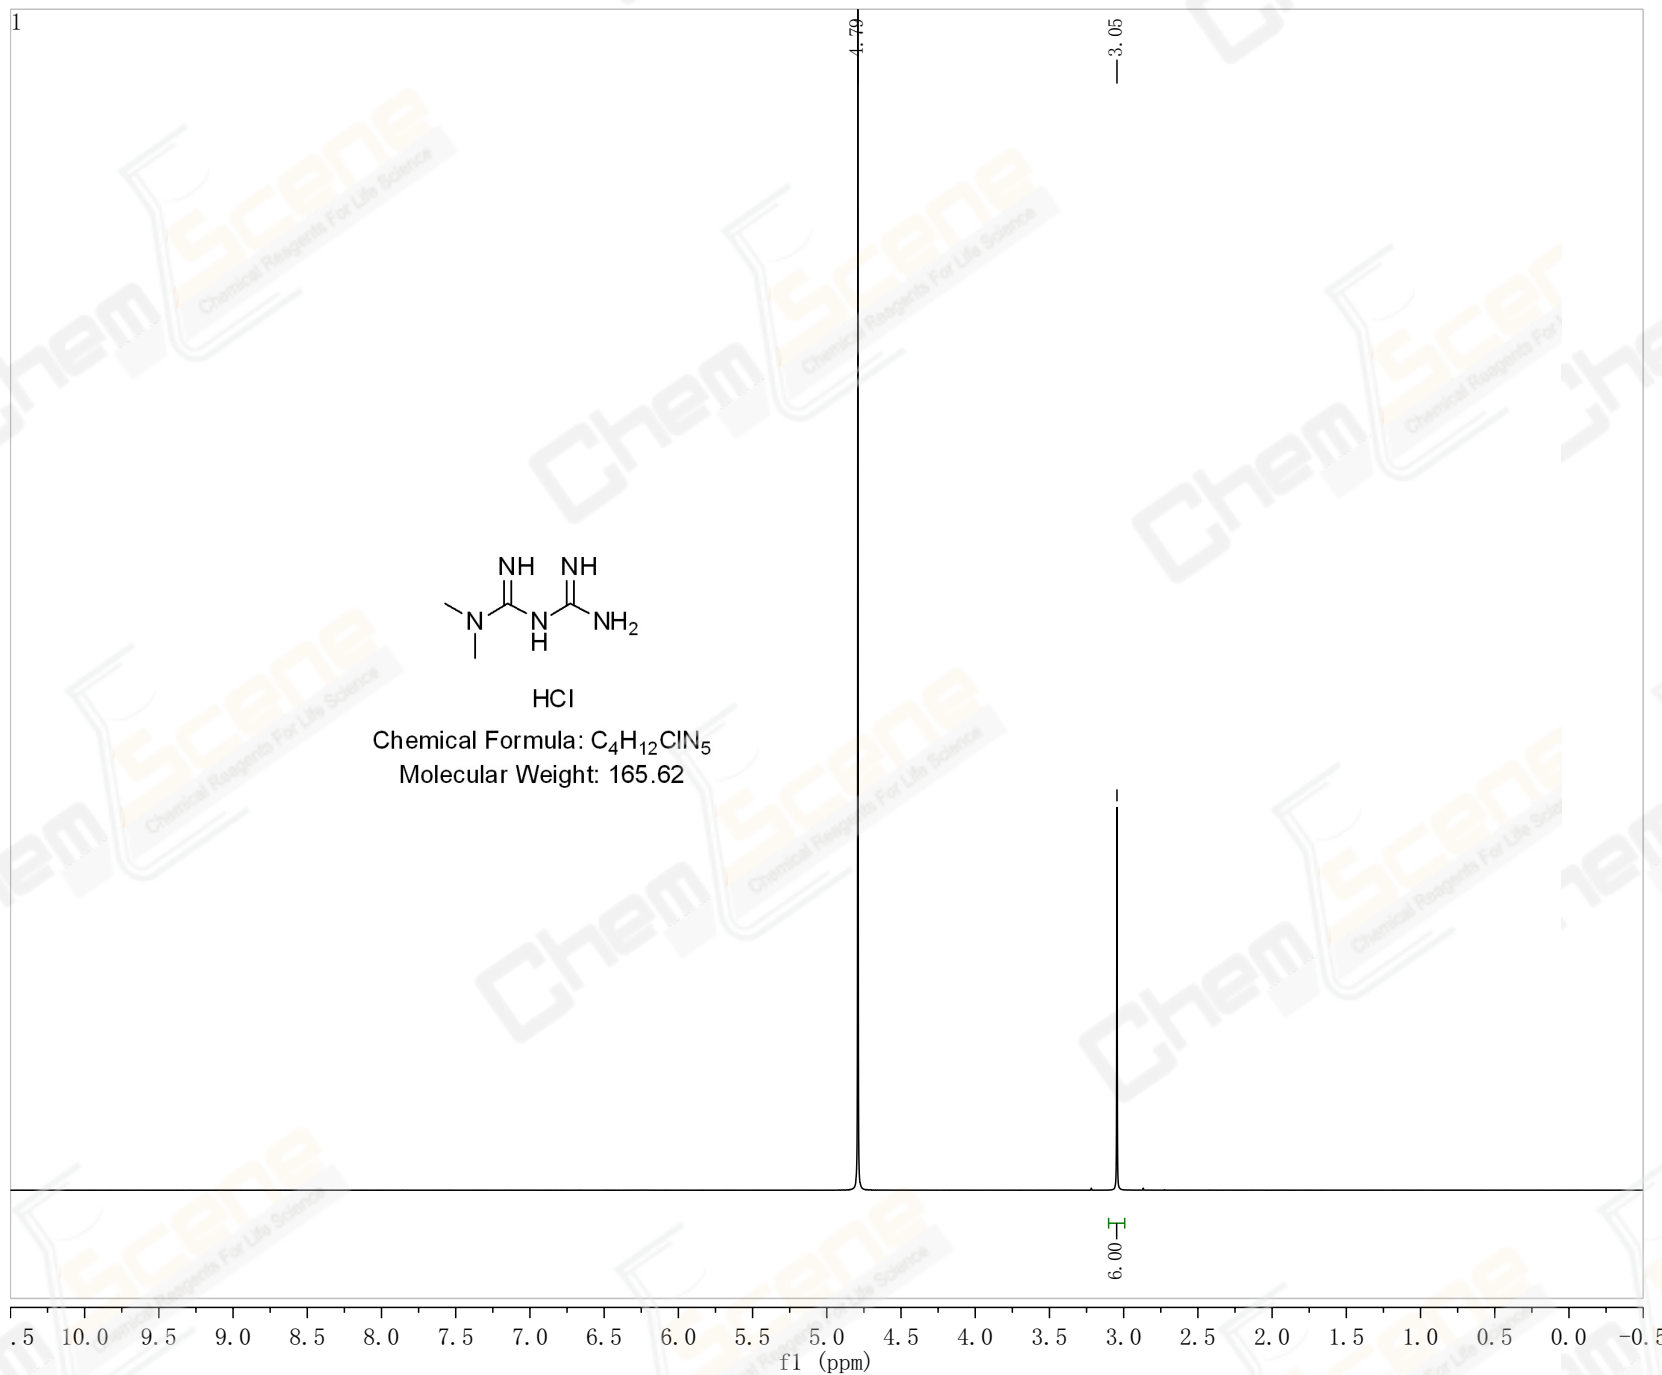

Parameter	Value
1 Title	1
2 Spectrometer	magnet
3 Solvent	D2O
4 Temperature	298.2
5 Pulse Sequence	slpul30
6 Experiment	1D
7 Number of Scans	16
8 Receiver Gain	64
9 Relaxation Delay	1.0000
10 Pulse Width	9.8000
11 Acquisition Time	3.9999
12 Acquisition Date	2024-03-13T13:46:44
13 Modification Date	2024-03-13T13:55:51
14 Spectrometer Frequency	400.00
15 Spectral Width	8108.0
16 Lowest Frequency	-1654.0
17 Nucleus	1H
18 Acquired Size	32431
19 Spectral Size	65536