


CAS NO.: 779353-01-4, CDCL3

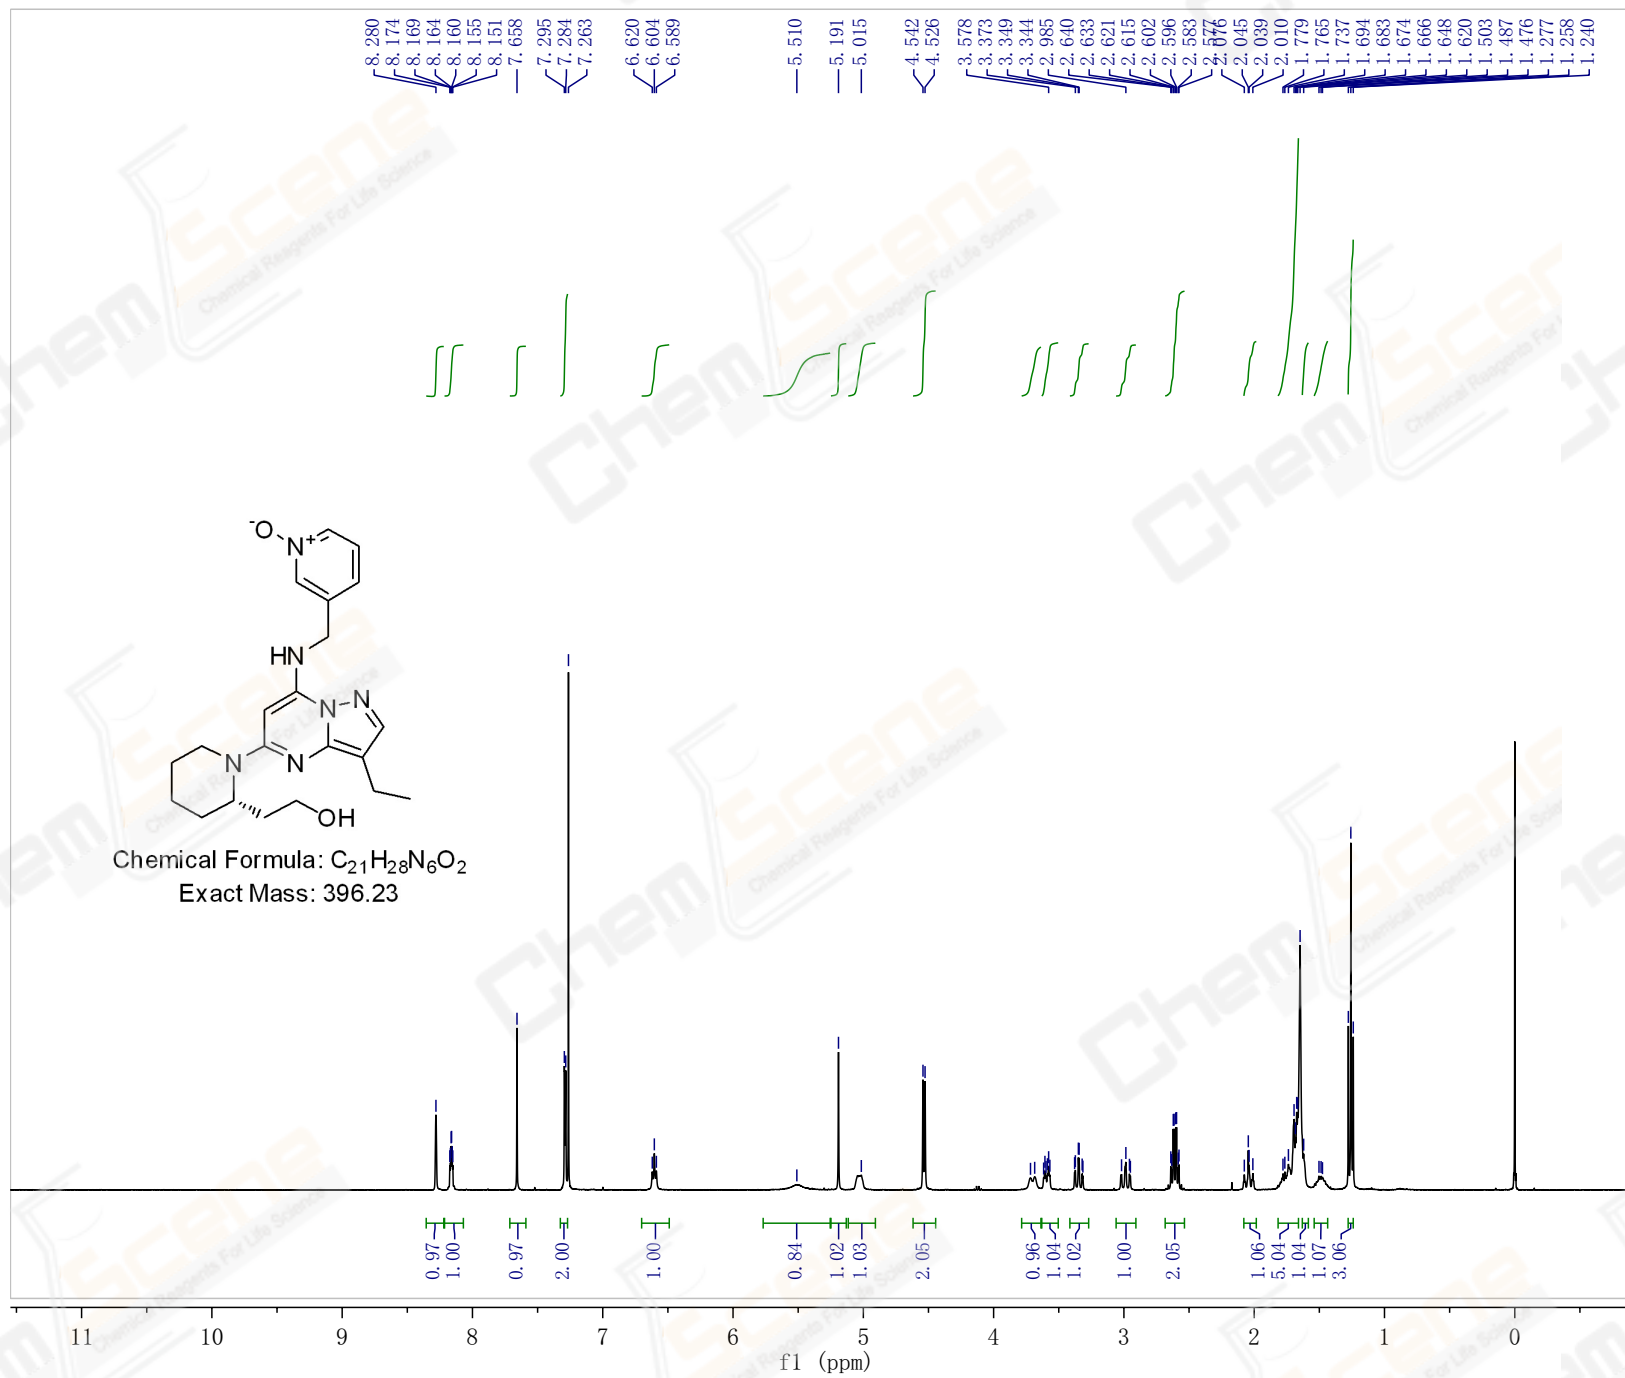

| Parameter | Value |
|---------------------------|---------------------|
| 1 Title | |
| 2 Origin | Bruker BioSpin GmbH |
| 3 Owner | nmrsu |
| 4 Spectrometer | Avance |
| 5 Solvent | CDCl3 |
| 6 Temperature | 298.9 |
| 7 Pulse Sequence | zg30 |
| 8 Experiment | 1D |
| 9 Number of Scans | 8 |
| 10 Receiver Gain | 101 |
| 11 Relaxation Delay | 1.0000 |
| 12 Pulse Width | 8.0000 |
| 13 Acquisition Time | 3.9977 |
| 14 Acquisition Date | 2022-09-01T09:03:51 |
| 15 Modification Date | 2022-09-01T09:07:59 |
| 16 Spectrometer Frequency | 400.13 |
| 17 Spectral Width | 8196.7 |
| 18 Lowest Frequency | -1636.0 |
| 19 Nucleus | 1H |
| 20 Acquired Size | 32768 |
| 21 Spectral Size | 65536 |