


CAS NO. : 139652-01-0, DMSO

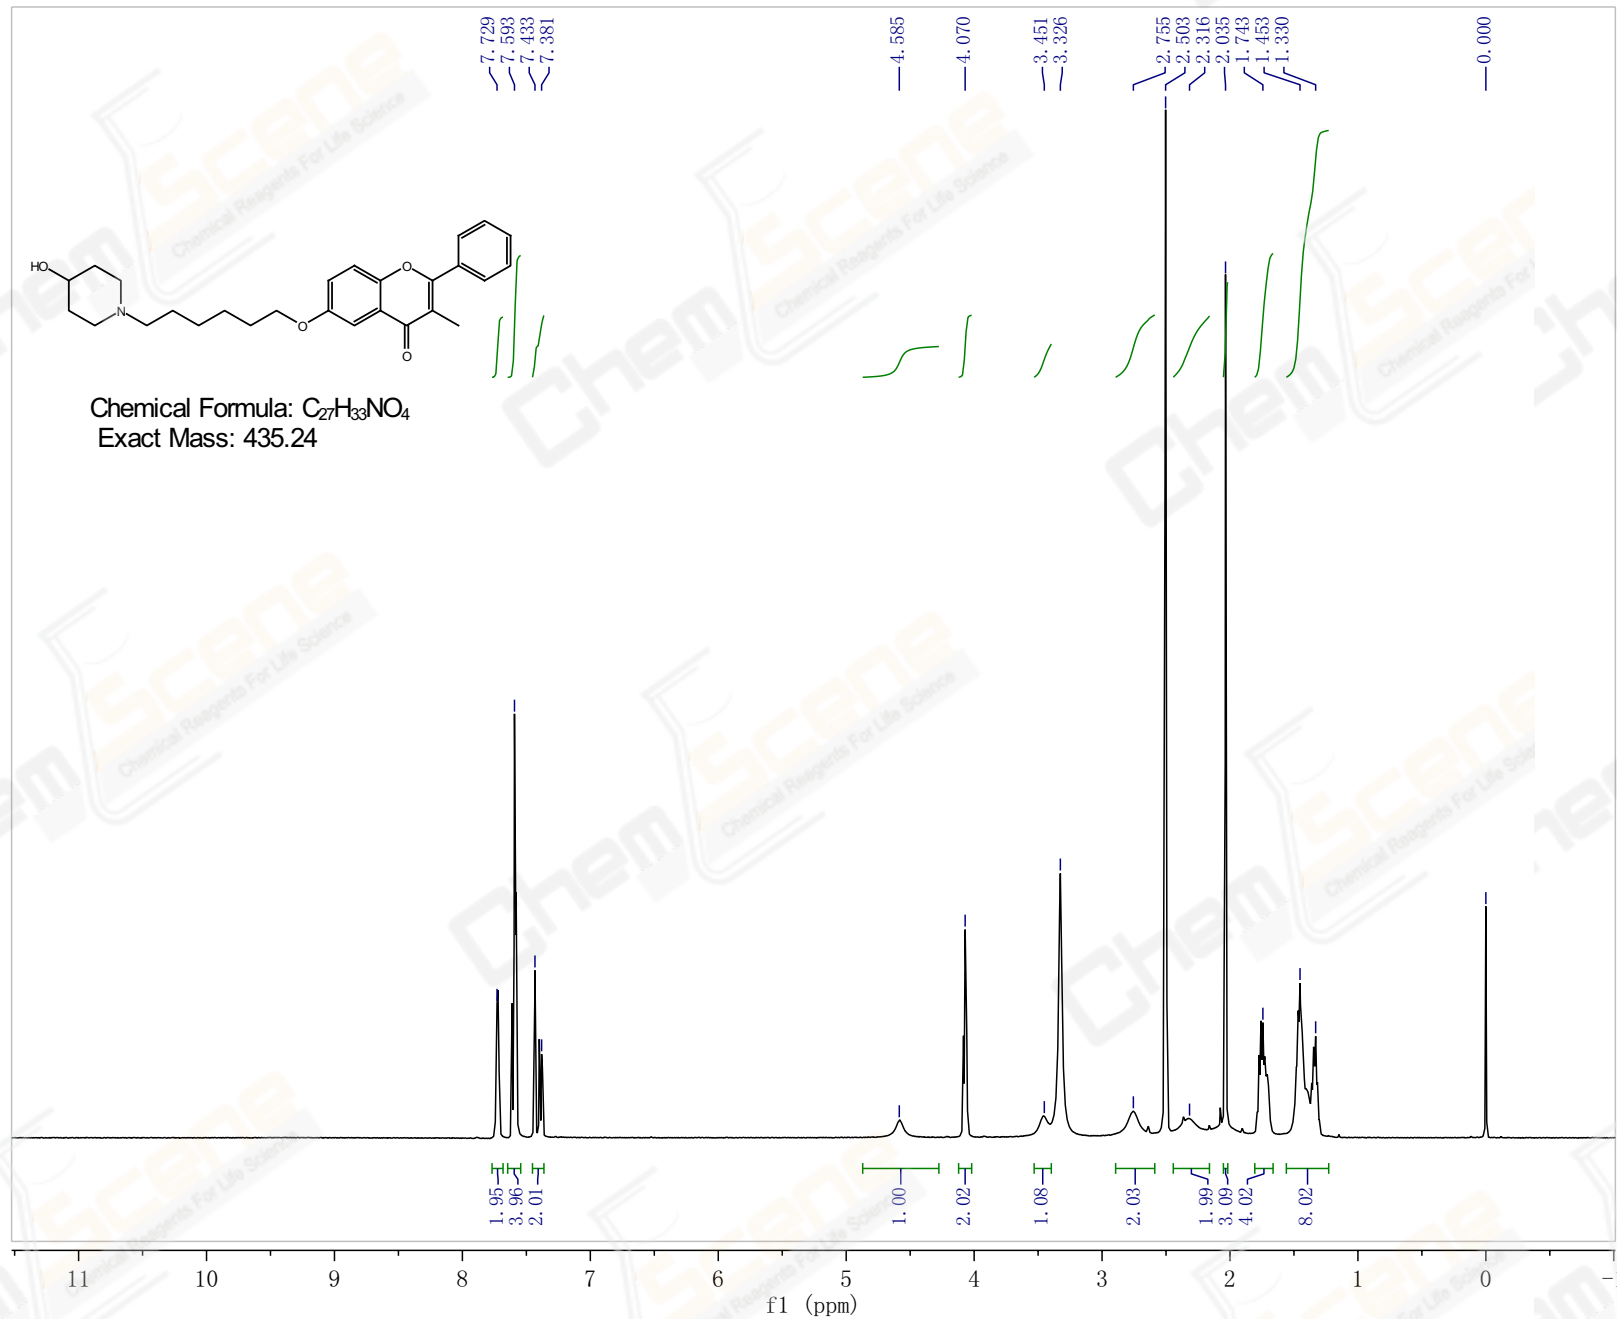

Parameter	Value
1 Data File Name	
2 Title	
3 Comment	
4 Origin	Bruker BioSpin GmbH
5 Owner	root
6 Site	
7 Spectrometer	Avance
8 Author	
9 Solvent	DMSO
10 Temperature	298.7
11 Pulse Sequence	zg30
12 Experiment	1D
13 Probe	Z119470_0328 (PA BBO 500S1 BBF-H-D-05 Z SP)
14 Number of Scans	16
15 Receiver Gain	101
16 Relaxation Delay	1.0000
17 Pulse Width	10.0000
18 Presaturation Frequency	
19 Acquisition Time	3.2768
20 Acquisition Date	2022-08-05T10:28:42
21 Modification Date	2022-08-05T10:28:42
22 Class	
23 Spectrometer	500.16