


CAS NO. : 2079895-62-6 DMSO

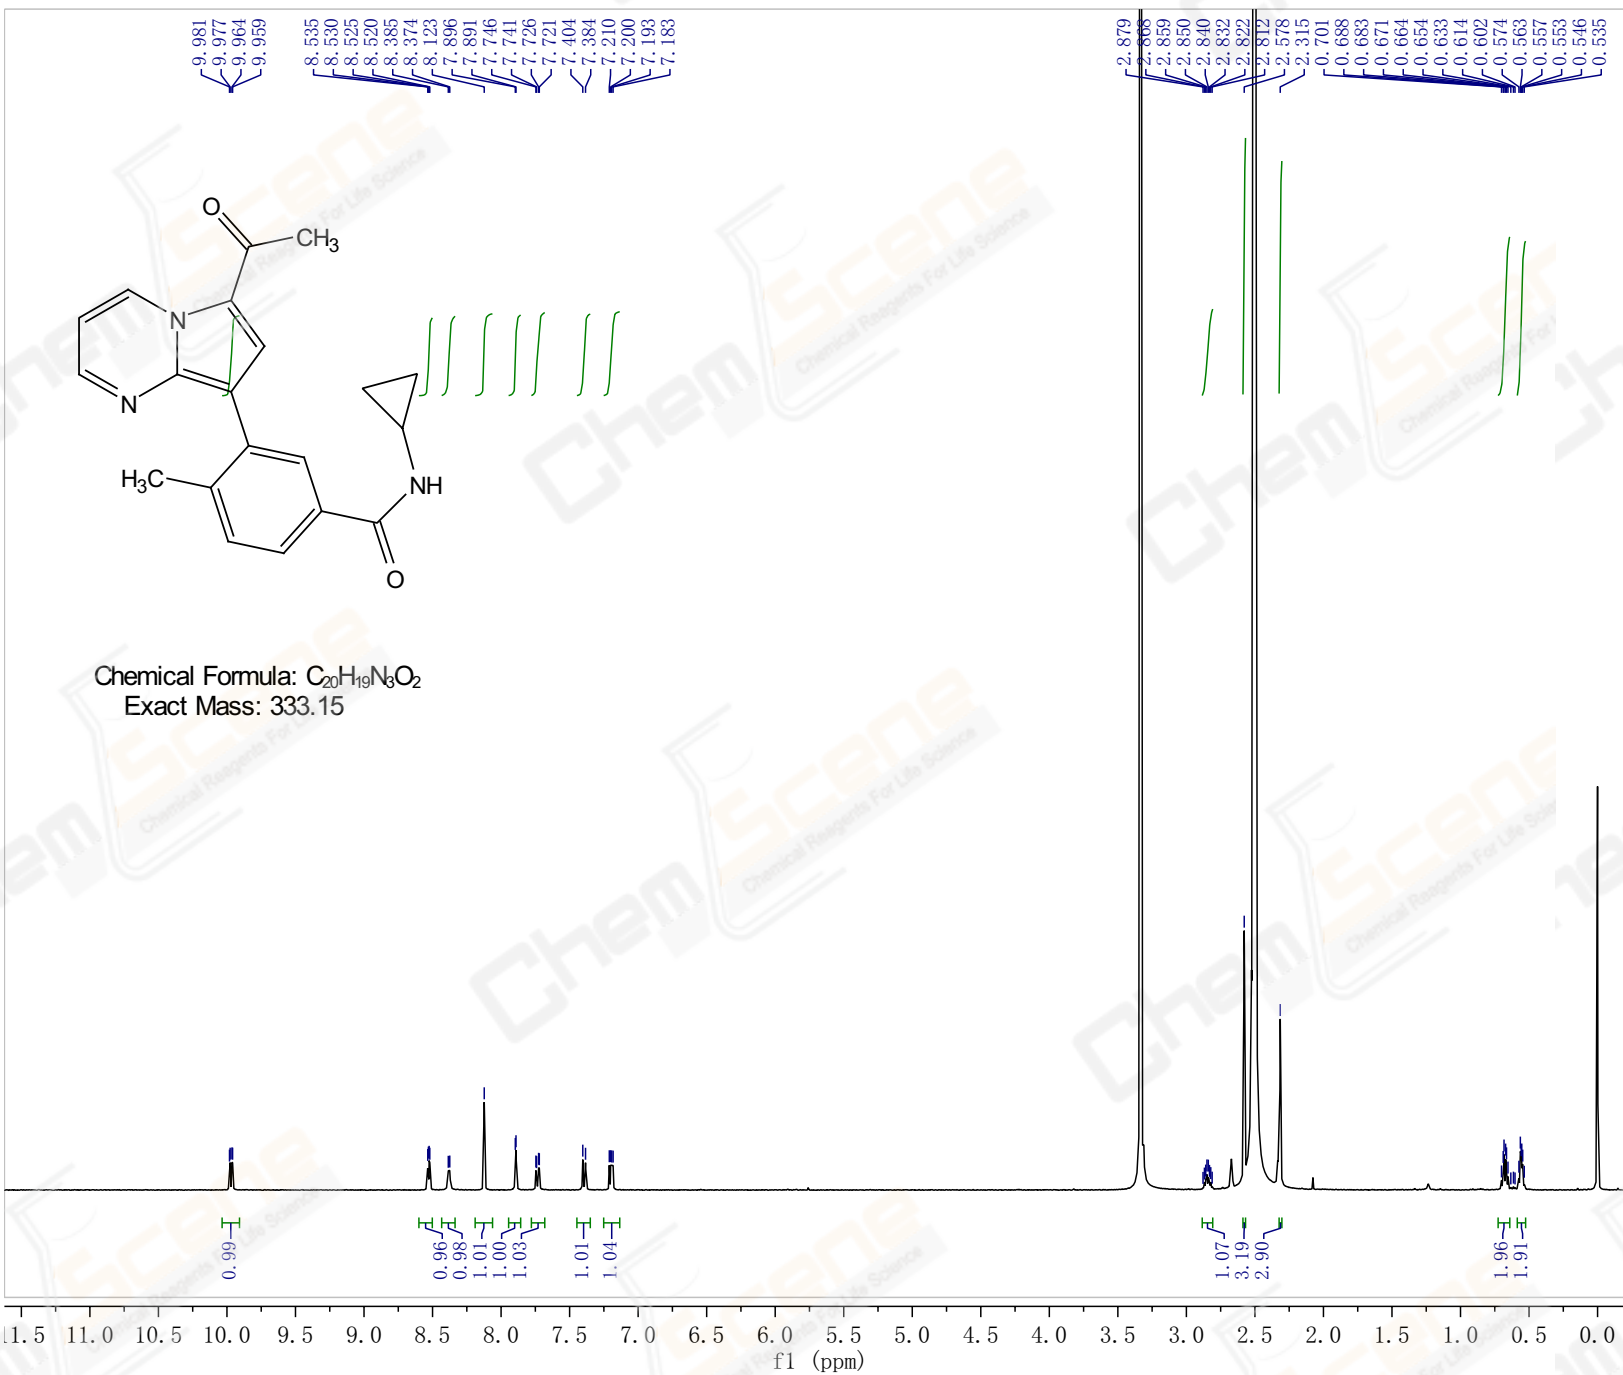

| Parameter | Value |
|----------------------------|--|
| 1 Data File Name | |
| 2 Title | 10.1.1r |
| 3 Comment | |
| 4 Origin | Bruker BioSpin GmbH |
| 5 Owner | nmr-su |
| 6 Site | |
| 7 Spectrometer | Default |
| 8 Author | |
| 9 Solvent | DMSO |
| 10 Temperature | 295.3 |
| 11 Pulse Sequence | zg30 |
| 12 Experiment | 1D |
| 13 Probe | Z163739_0572 (PI HR- BBO400S1-BBF/ H/ D-5.0-Z SP) |
| 14 Number of Scans | 32 |
| 15 Receiver Gain | 101 |
| 16 Relaxation Delay | 1.0000 |
| 17 Pulse Width | 8.0000 |
| 18 Presaturation Frequency | |
| 19 Acquisition Time | 3.9977 |
| 20 Acquisition Date | 2022-09-29T10:06:45 |
| 21 Modification Date | 2022-09-29T10:06:36 |
| 22 Class | |
| 23 Spectrometer Frequency | 400.13 |
| 24 Spectral Width | 8196.7 |
| 25 Lowest Frequency | -1629.1 |
| 26 Nucleus | 1H |
| 27 Acquired Size | 32768 |
| 28 Spectral Size | 65536 |