


CAS NO.: 1802425-99-5 ,CD3OD

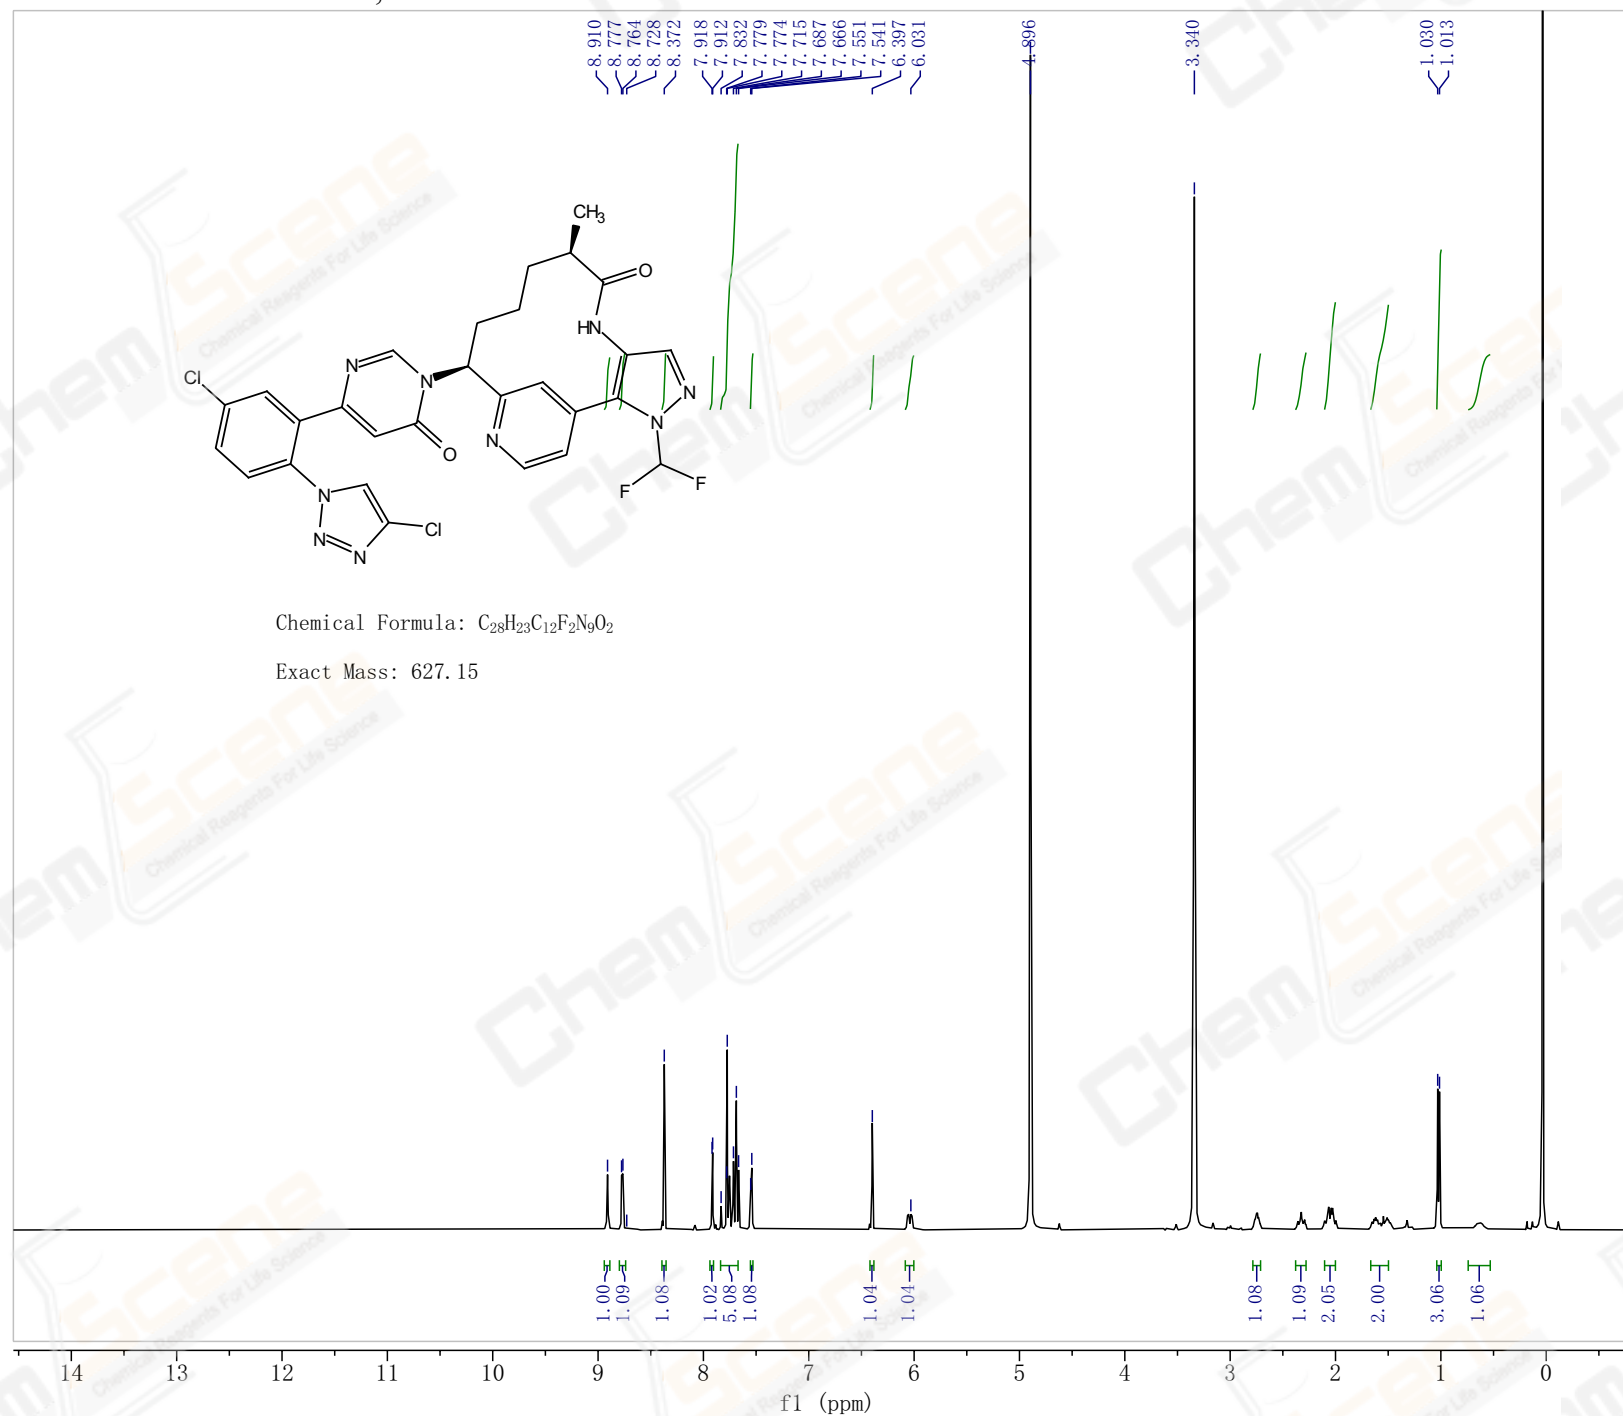

Parameter	
1 Data File Name	/ /
2 标题	nmrsu/ nmr/ YT-131- TM-1018/ 10/ pdata/ 1/ 1r
3 Comment	YT-131- TM-1018. 10. 1. 1r
4 Origin	Bruker BioSpin GmbH
5 Owner	nmrsu
6 Site	
7 Instrument	Default
8 Author	
9 Solvent	CD3OD_SPE
10 Temperature	297.2
11 Pulse Sequence	zg30
12 Experiment	1D
13 Probe	Z163739_0572 (PI HR-BB0400S1-BBF/ H/ D-5. 0-Z SP)
14 Number of Scans	32
15 Receiver Gain	101.0
16 Relaxation Delay	1.0000
17 Pulse Width	8.0000
18 Presaturation Frequency	
19 Acquisition Time	3.9977
20 Acquisition Date	2022-10-18T09:17:14
21 Modification Date	2022-10-18T09:17:52
22 Class	
23 Spectrometer Frequency	400.13