


CAS NO.: 2079895-62-6,DMSO

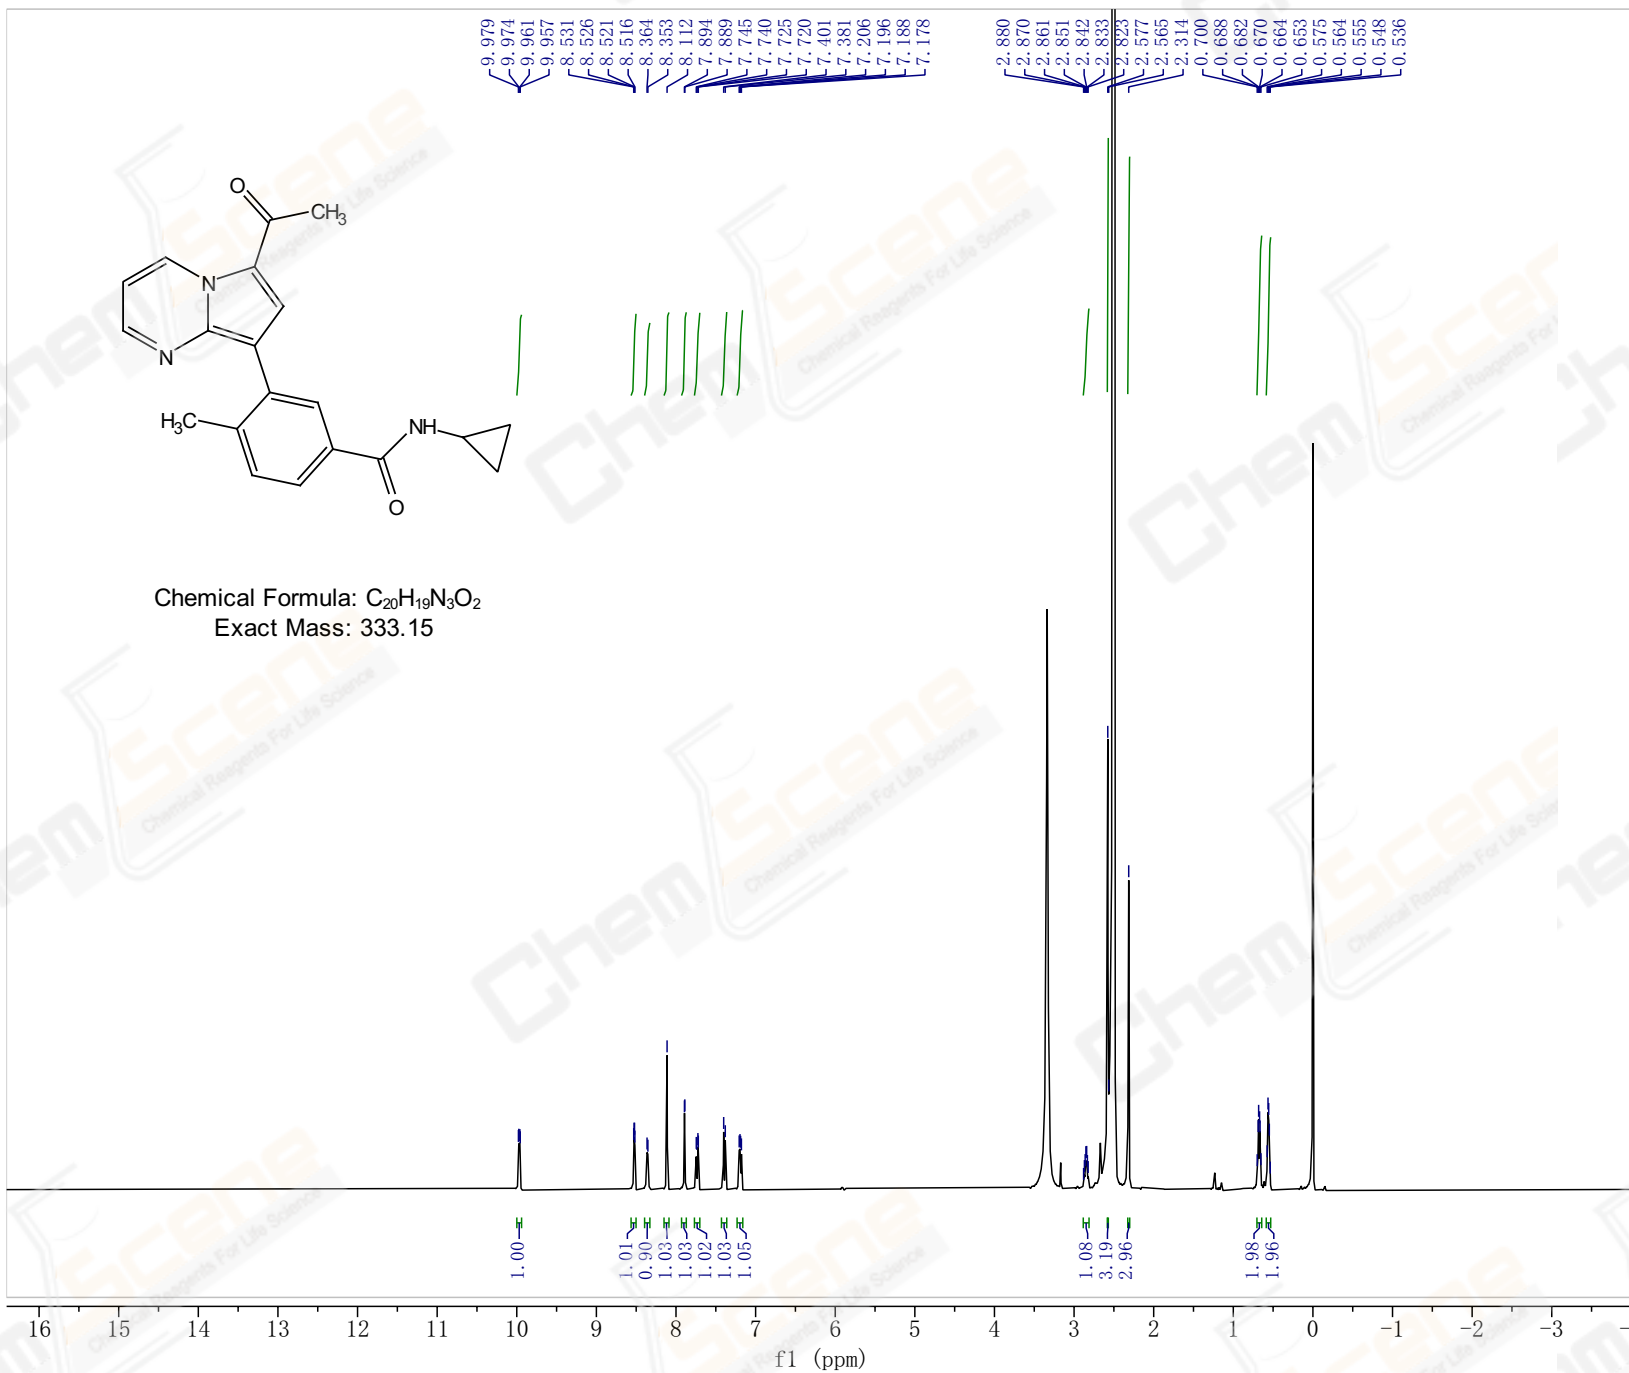

Parameter	Value
1 Data File Name	
2	
3 Comment	
4 Origin	Bruker BioSpin GmbH
5 Owner	nmrsu
6 Site	
7 Instrument	Avance
8 Author	
9 Solvent	DMSO
10 Temperature	300.0
11 Pulse Sequence	zg30
12 Experiment	1D
13 Probe	Z163739_0572 (PI HR-BB0400S1-BBF/H/ D-5.0-Z SP)
14 Number of Scans	32
15 Receiver Gain	101.0
16 Relaxation Delay	1.0000
17 Pulse Width	8.0000
18 Presaturation Frequency	
19 Acquisition Time	3.9977
20 Acquisition Date	2022-11-08T15:14:20
21 Modification Date	2022-11-08T15:15:45
22 Class	
23 Spectrometer Frequency	400.13
24 Spectral Width	8196.7
25 Lowest Frequency	-1630.3
26 Nucleus	1H
27 Acquired Size	32768