


CAS NO.: 8002-43-5, CDCL3

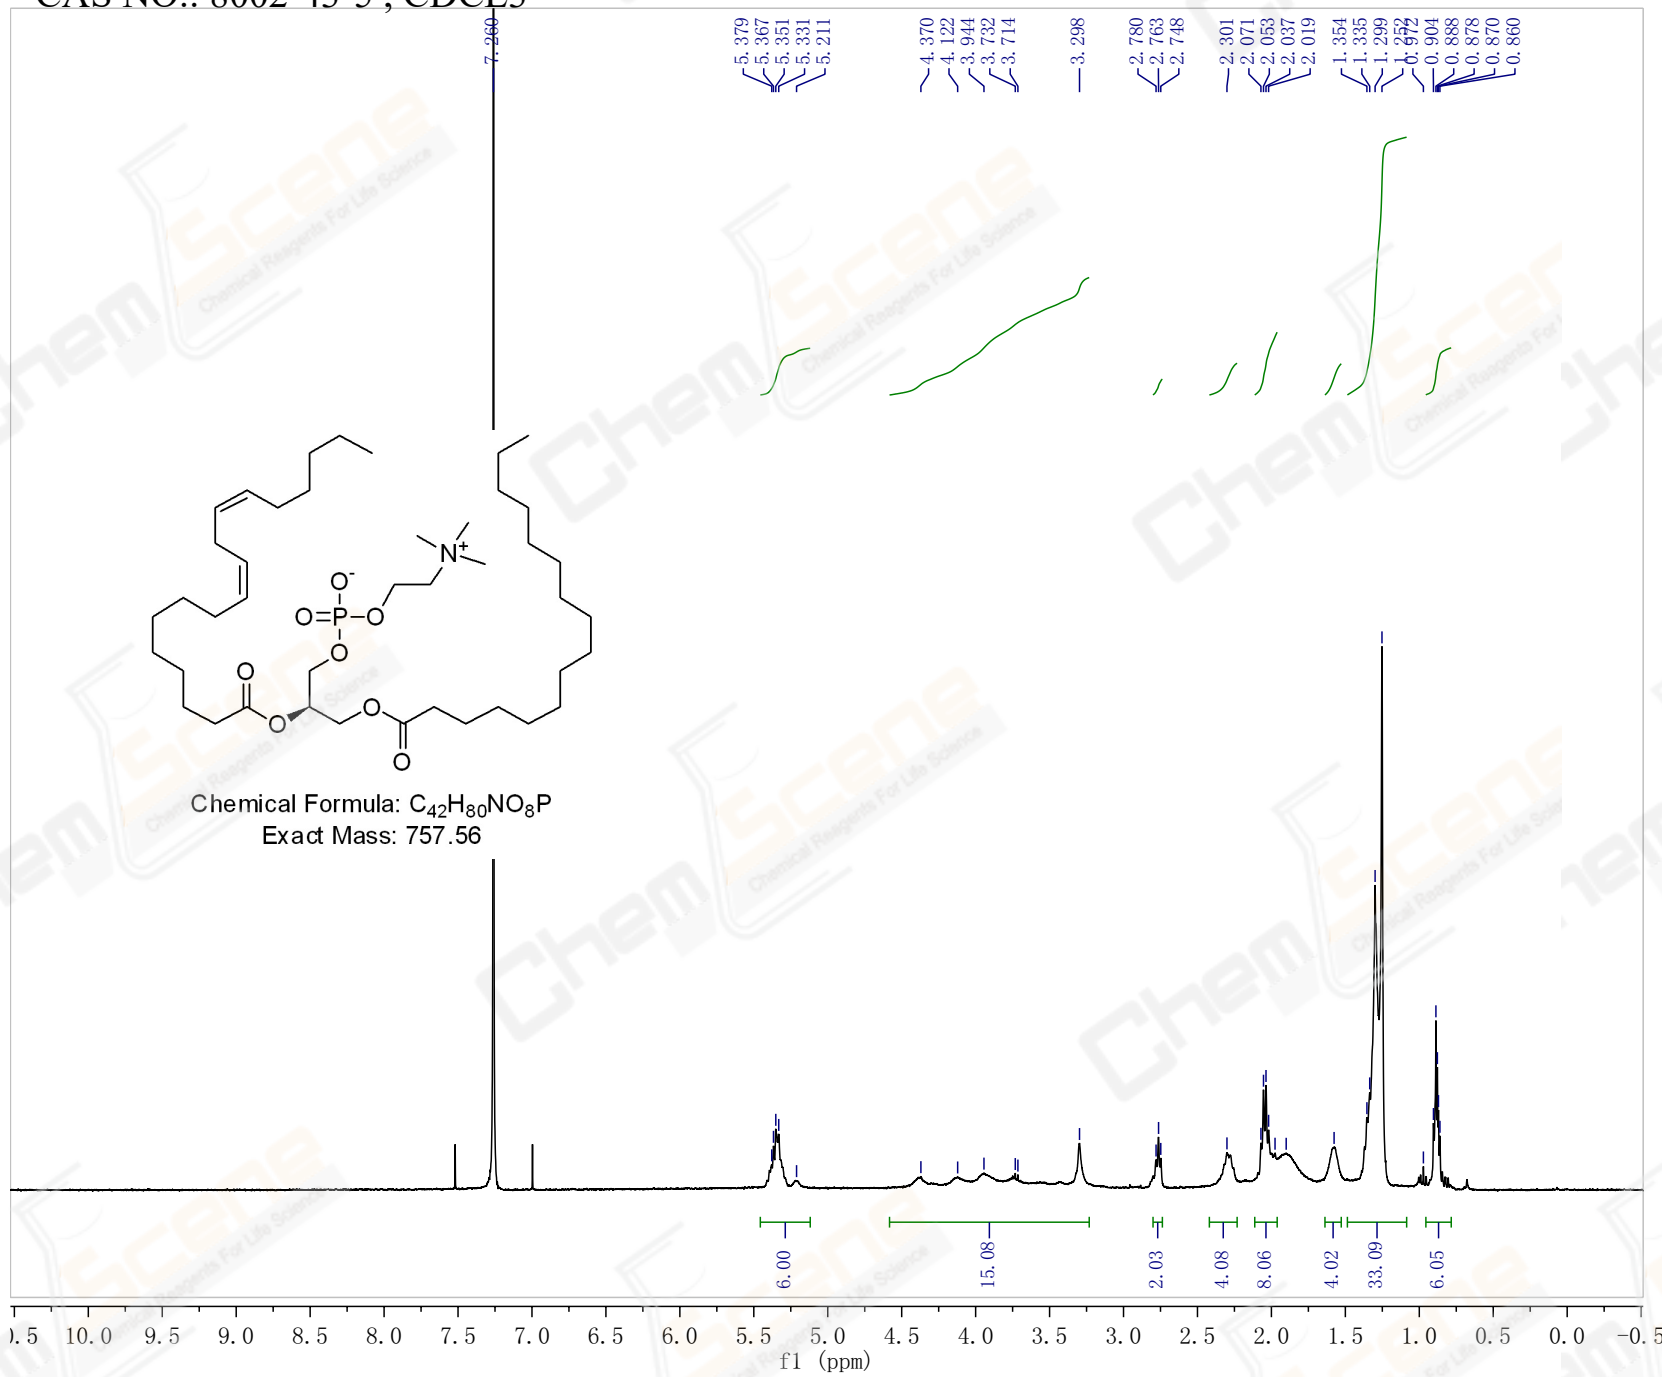

| Parameters | |
|---------------------------|---------------------|
| Parameter | Value |
| 1 Title | |
| 2 Spectrometer | Avance |
| 3 Solvent | CDCL3 |
| 4 Temperature | 298.2 |
| 5 Pulse Sequence | zg30 |
| 6 Number of Scans | 8 |
| 7 Receiver Gain | 101 |
| 8 Relaxation Delay | 1.0000 |
| 9 Pulse Width | 8.0000 |
| 10 Acquisition Time | 3.9977 |
| 11 Acquisition Date | 2022-12-30T19:00:48 |
| 12 Modification Date | 2022-12-30T19:06:17 |
| 13 Spectrometer Frequency | 400.13 |
| 14 Spectral Width | 8196.7 |
| 15 Lowest Frequency | -1627.6 |
| 16 Nucleus | 1H |
| 17 Acquired Size | 32768 |
| 18 Spectral Size | 65536 |