


CAS NO.: 8002-43-5, CDCl₃

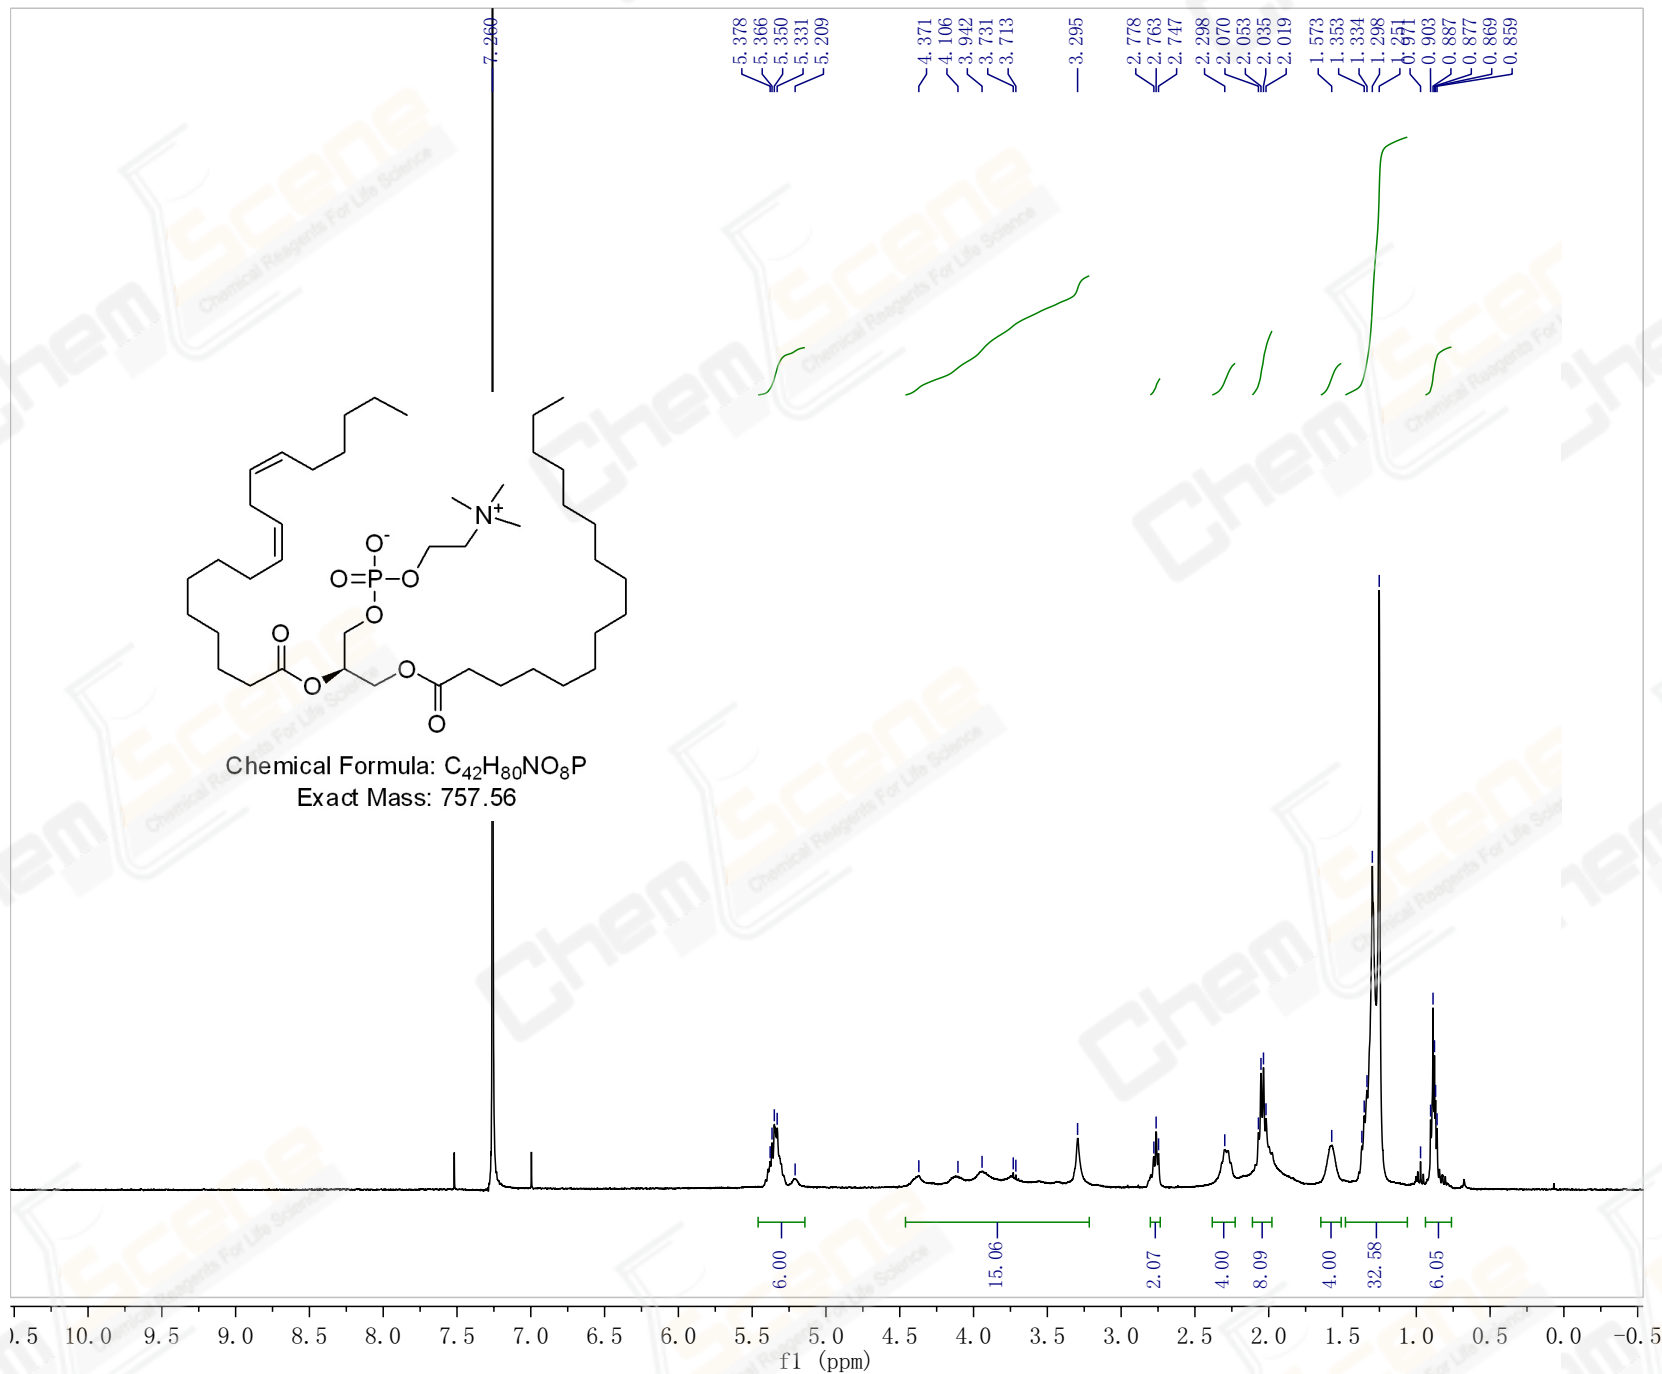

Parameters	
Parameter	Value
1	Title
2	Spectrometer Avance
3	Solvent CDCl ₃
4	Temperature 298.2
5	Pulse Sequence zg30
6	Number of Scans 8
7	Receiver Gain 101
8	Relaxation Delay 1.0000
9	Pulse Width 8.0000
10	Acquisition Time 3.9977
11	Acquisition Date 2022-12-30T19:05:35
12	Modification Date 2022-12-30T19:11:04
13	Spectrometer Frequency 400.13
14	Spectral Width 8196.7
15	Lowest Frequency -1664.7
16	Nucleus 1H
17	Acquired Size 32768
18	Spectral Size 65536