


CAS NO.: 518-75-2, CDCL3

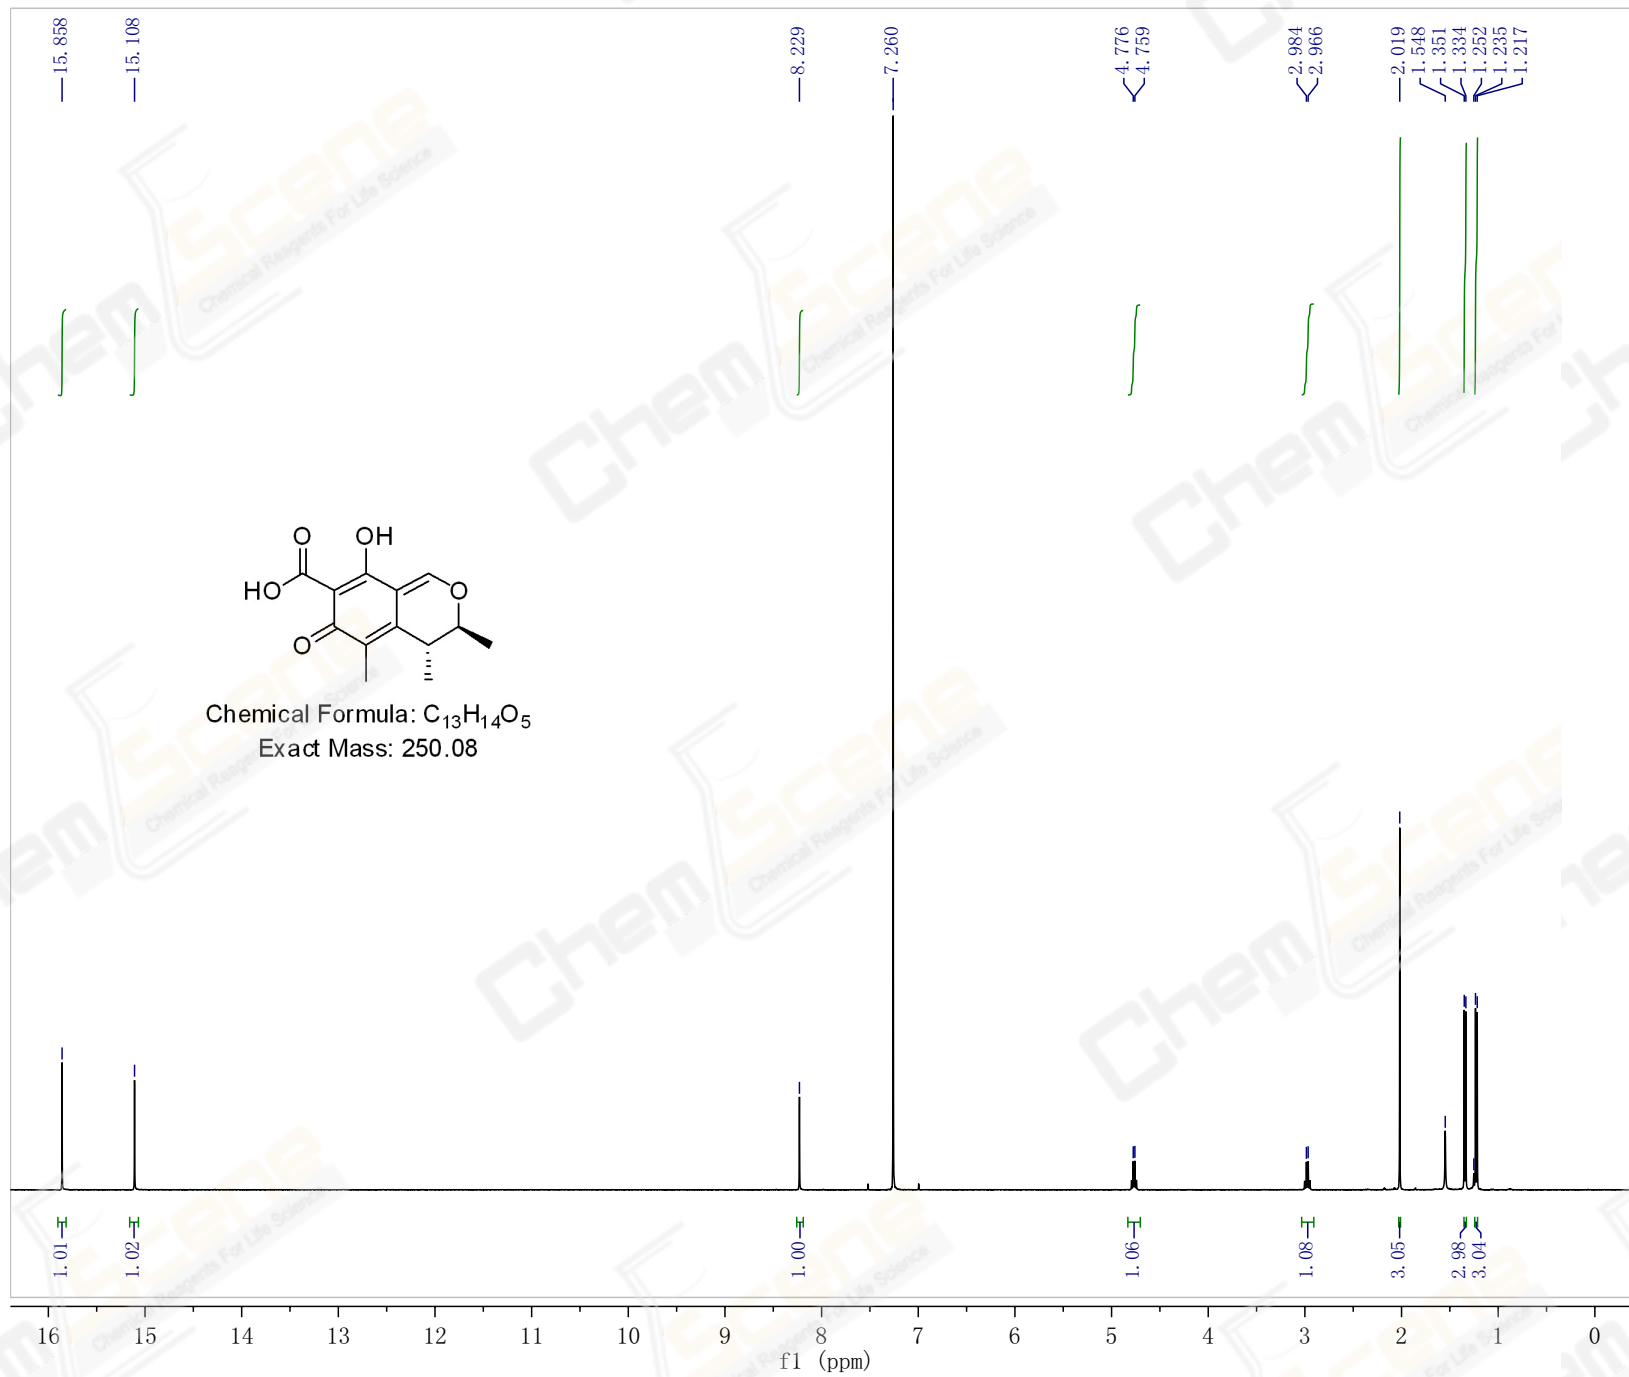

Parameters		
Parameter	Value	
1	Title	
2	Spectrometer	Avance
3	Solvent	CDCL3
4	Temperature	298.2
5	Pulse Sequence	zg30
6	Number of Scans	8
7	Receiver Gain	101
8	Relaxation Delay	1.0000
9	Pulse Width	8.0000
10	Acquisition Time	3.9977
11	Acquisition Date	2023-01-06T11:14:10
12	Modification Date	2023-01-06T11:19:38
13	Spectrometer Frequency	400.13
14	Spectral Width	8196.7
15	Lowest Frequency	-1627.6
16	Nucleus	1H
17	Acquired Size	32768
18	Spectral Size	65536