


CAS NO.: 941678-49-5, DMSO

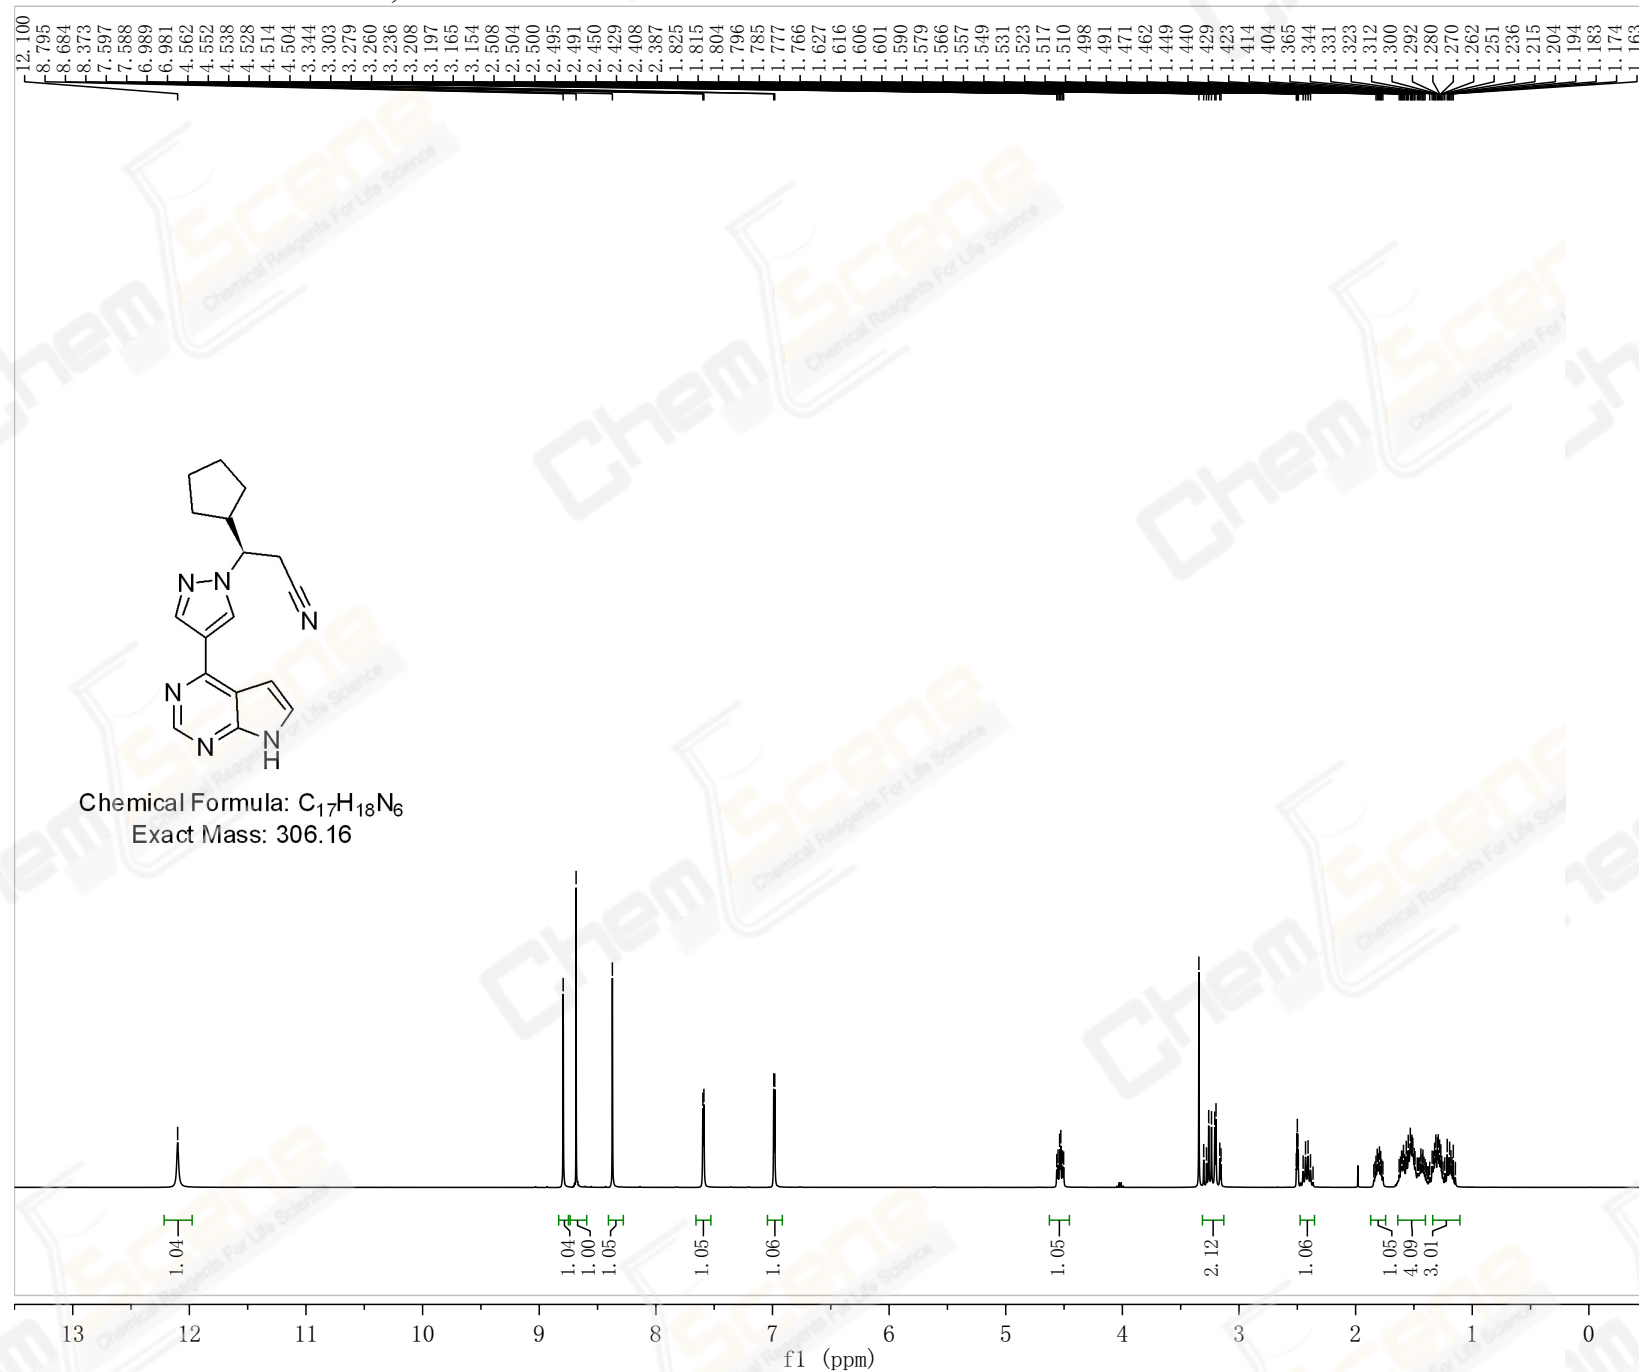

Parameter	Value
1 Title	
2 Spectrometer	Avance neo 400
3 Solvent	DMSO
4 Temperature	298.1
5 Pulse Sequence	zg30
6 Experiment	1D
7 Number of Scans	8
8 Receiver Gain	72
9 Relaxation Delay	1.0000
10 Pulse Width	8.0000
11 Acquisition Time	3.9977
12 Acquisition Date	2023-12-06T05:23:15
13 Modification Date	2023-12-06T05:32:59
14 Spectrometer Frequency	400.14
15 Spectral Width	8196.7
16 Lowest Frequency	-1622.7
17 Nucleus	1H
18 Acquired Size	32768
19 Spectral Size	65536