


CAS NO.: 86811-36-1 ,CDCL3

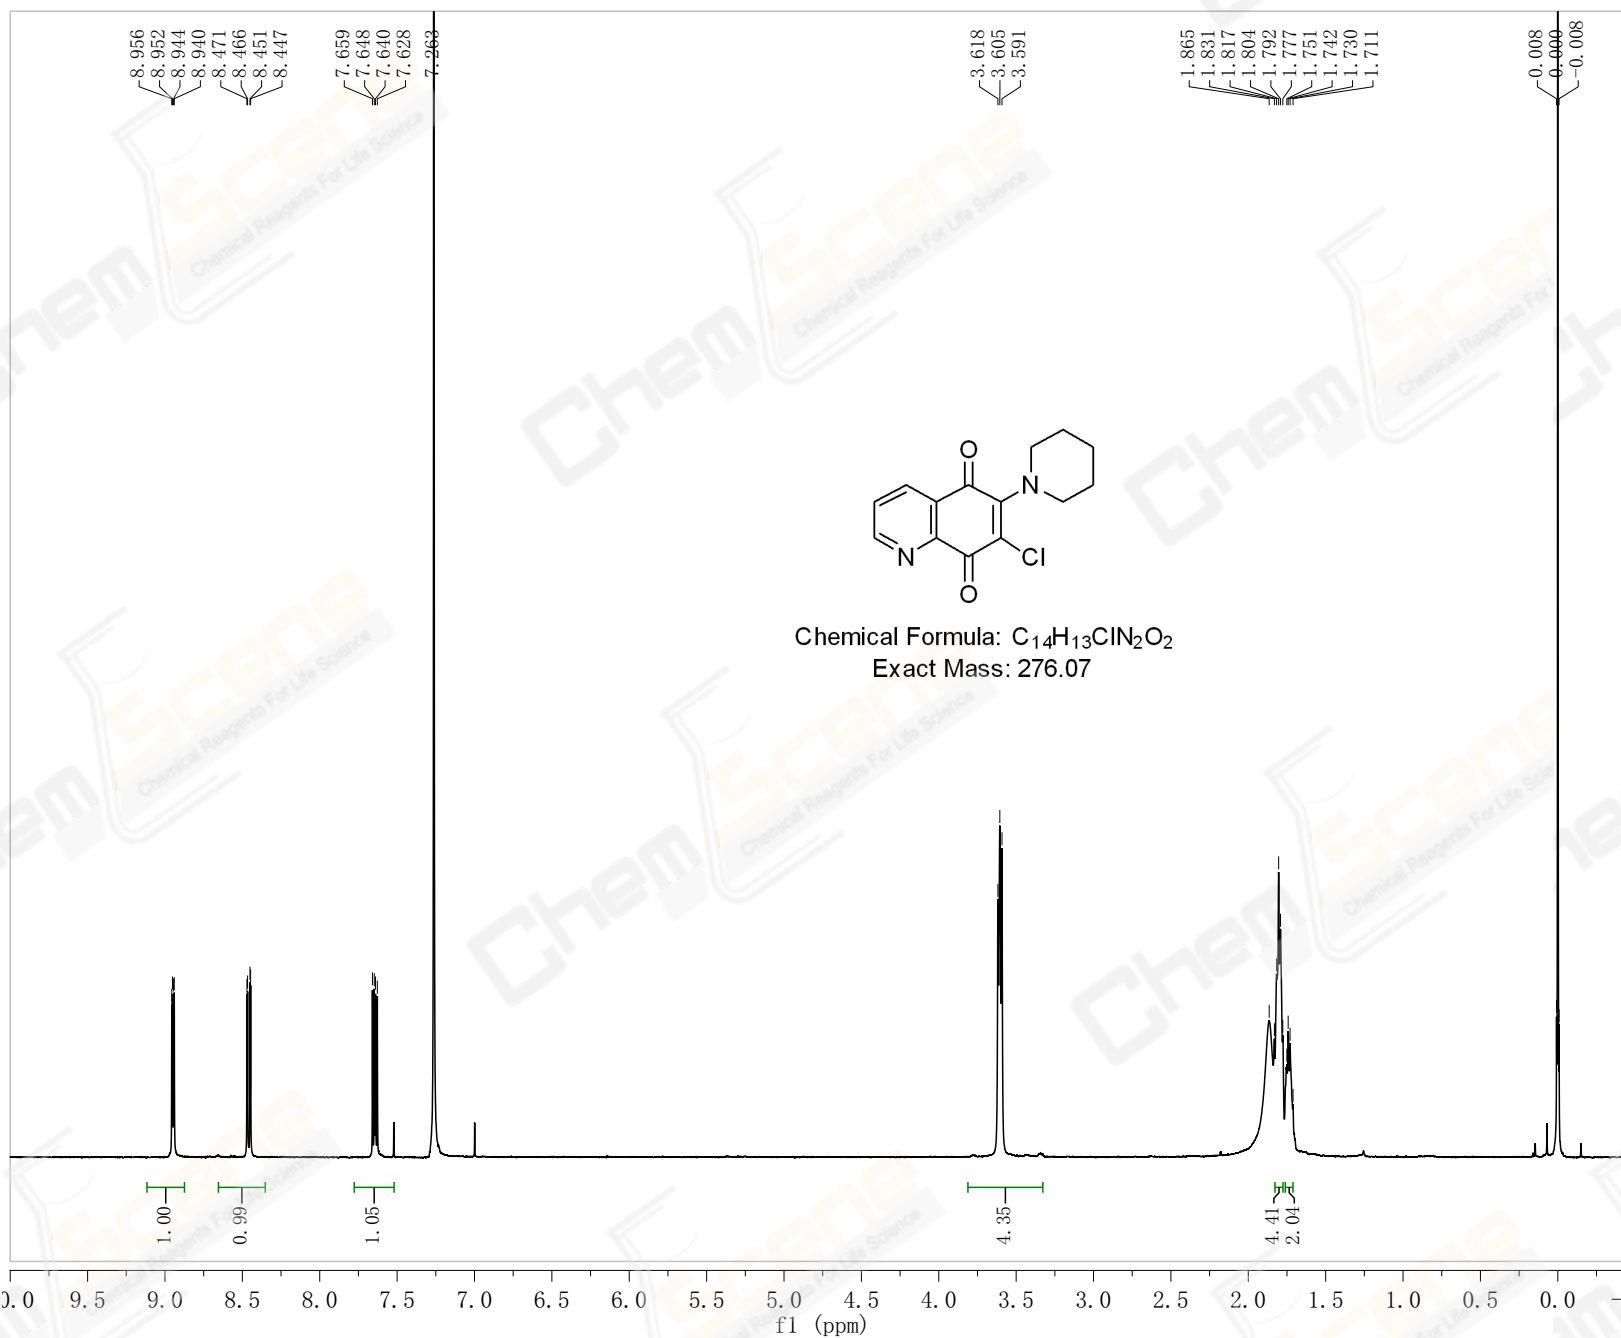

| Parameter | Value |
|---------------------------|------------------------------------|
| 1 Data File Name | / |
| 2 Title | HNMR-HD-466-300MG |
| 3 Comment | {PROTON 8} CDC13 {D:\data} root 21 |
| 4 Origin | Bruker BioSpin GmbH |
| 5 Owner | root |
| 6 Site | |
| 7 Spectrometer | Avance neo 400 |
| 8 Author | |
| 9 Solvent | CDCl3 |
| 10 Temperature | 298.2 |
| 11 Pulse Sequence | zg30 |
| 12 Experiment | 1D |
| 13 Number of Scans | 8 |
| 14 Receiver Gain | 101 |
| 15 Relaxation Delay | 1.0000 |
| 16 Pulse Width | 8.0000 |
| 17 Acquisition Time | 3.9977 |
| 18 Acquisition Date | 2023-04-25T11:42:27 |
| 19 Modification Date | 2023-04-25T11:45:22 |
| 20 Spectrometer Frequency | 400.14 |
| 21 Spectral Width | 8196.7 |
| 22 Lowest Frequency | -1636.1 |
| 23 Nucleus | 1H |
| 24 Acquired Size | 32768 |

Supervisor:

Operator:

Date: