


CAS NO.: 2627-69-2, DMSO

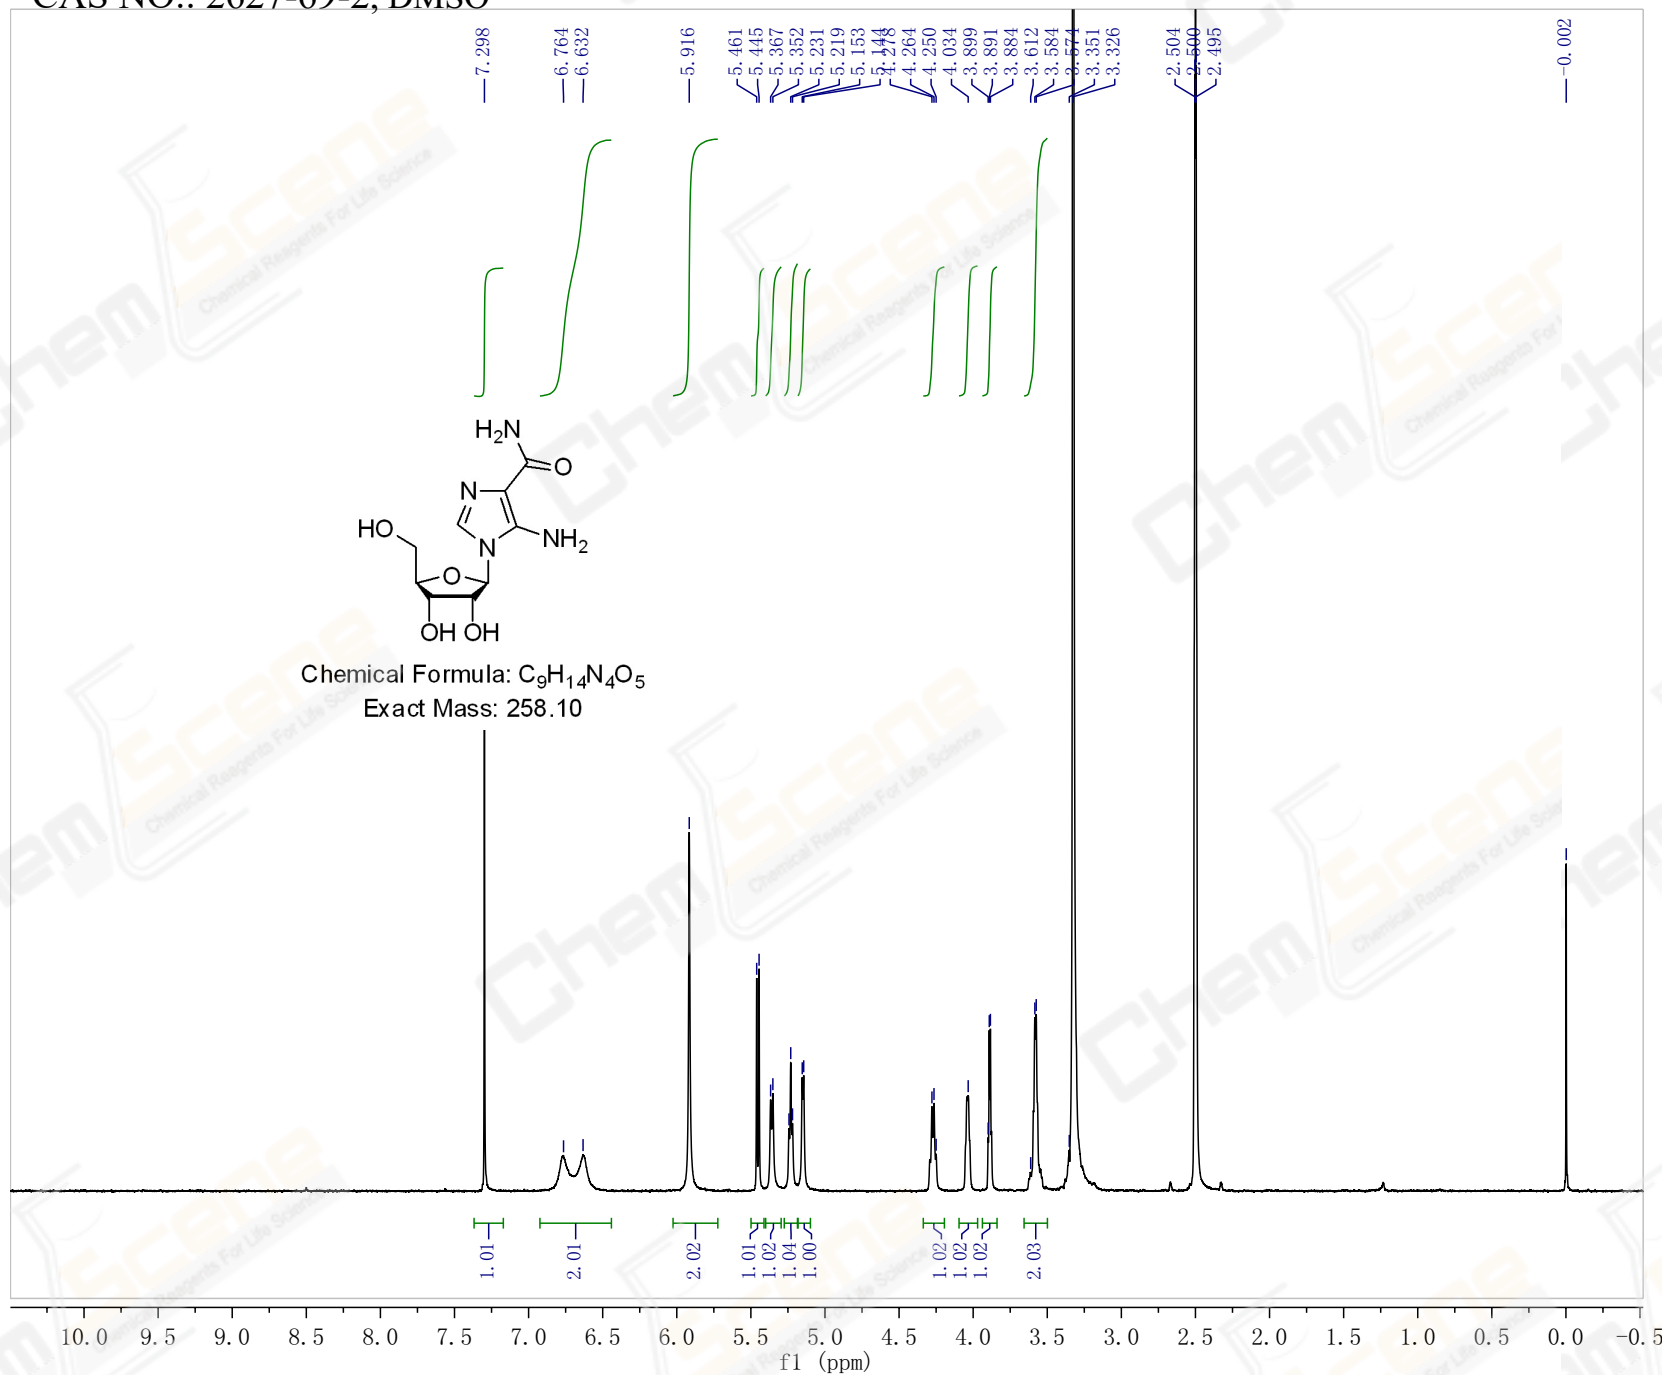

Parameter	Value
1 Title	
2 Origin	Bruker BioSpin GmbH
3 Owner	nmrsu
4 Spectrometer	Avance
5 Solvent	DMSO
6 Temperature	298.3
7 Pulse Sequence	zg30
8 Experiment	1D
9 Number of Scans	8
10 Receiver Gain	101
11 Relaxation Delay	1.0000
12 Pulse Width	8.0000
13 Acquisition Time	3.9977
14 Acquisition Date	2023-07-27T12:26:27
15 Modification Date	2023-07-27T12:33:22
16 Spectrometer Frequency	400.13
17 Spectral Width	8196.7
18 Nucleus	$^1H$