


CAS NO.: 153-91-3, MeOD

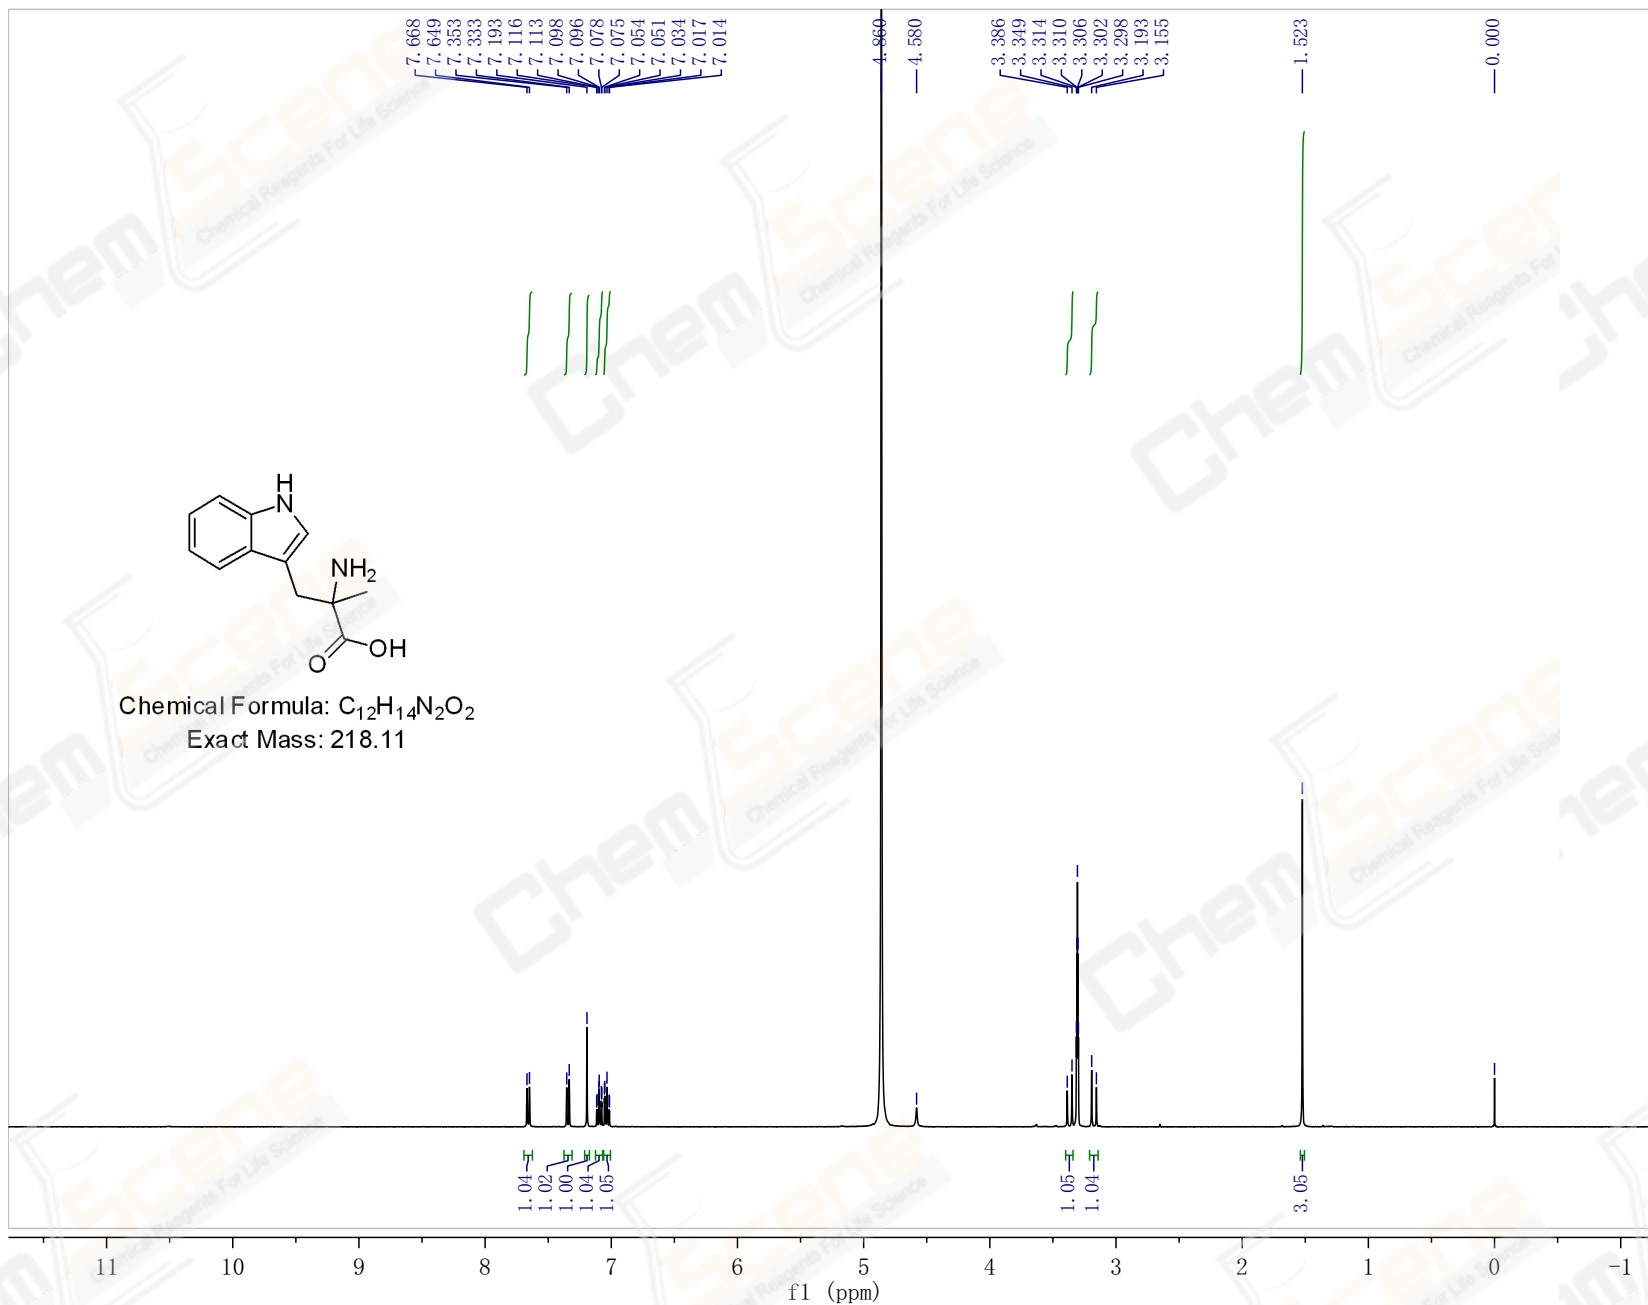

Parameter	Value
1 Title	
2 Spectrometer	Avance
3 Solvent	MeOD
4 Temperature	298.2
5 Pulse Sequence	zg30
6 Number of Scans	8
7 Receiver Gain	101
8 Relaxation Delay	1.0000
9 Pulse Width	8.0000
10 Acquisition Time	3.9977
11 Acquisition Date	2023-11-03T13:53:29
12 Modification Date	2023-11-03T14:01:36
13 Spectrometer Frequency	400.13
14 Spectral Width	8196.7
15 Lowest Frequency	-1637.1
16 Nucleus	$^1H$
17 Acquired Size	32768
18 Spectral Size	65536