


CAS NO.: 117591-20-5, CDCL3

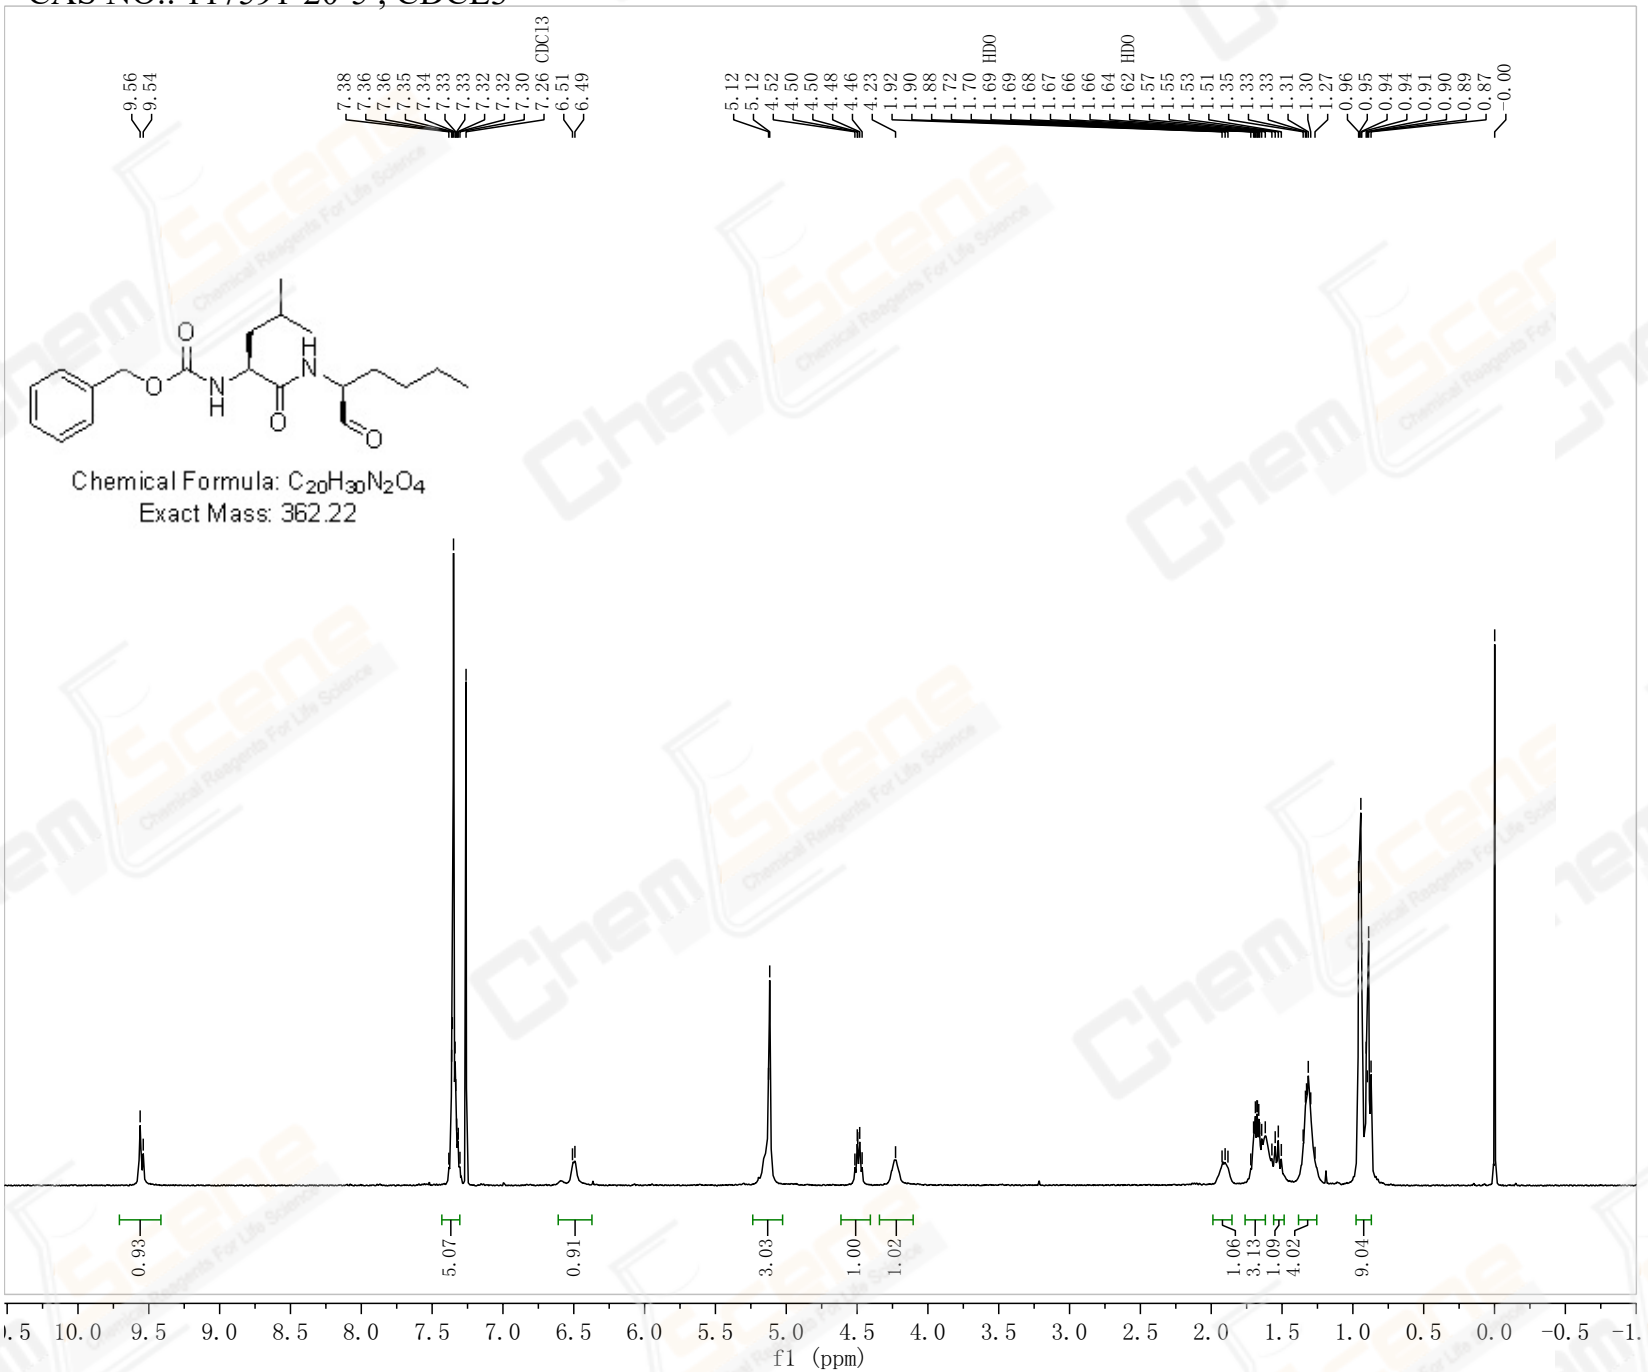

Parameter	Value
1 Title	
2 Spectrometer	magnet
3 Solvent	CDCl3
4 Temperature	296.4
5 Pulse Sequence	slpul30
6 Experiment	1D
7 Number of Scans	16
8 Receiver Gain	64
9 Relaxation Delay	1.0000
10 Pulse Width	9.8000
11 Acquisition Time	3.9999
12 Acquisition Date	2024-03-29T13:44:38
13 Modification Date	2024-03-29T13:54:46
14 Spectrometer Frequency	400.00
15 Spectral Width	8108.0
16 Lowest Frequency	-1670.7
17 Nucleus	1H
18 Acquired Size	32431
19 Spectral Size	65536