


CAS NO.: 153874-14-7, CDCL3

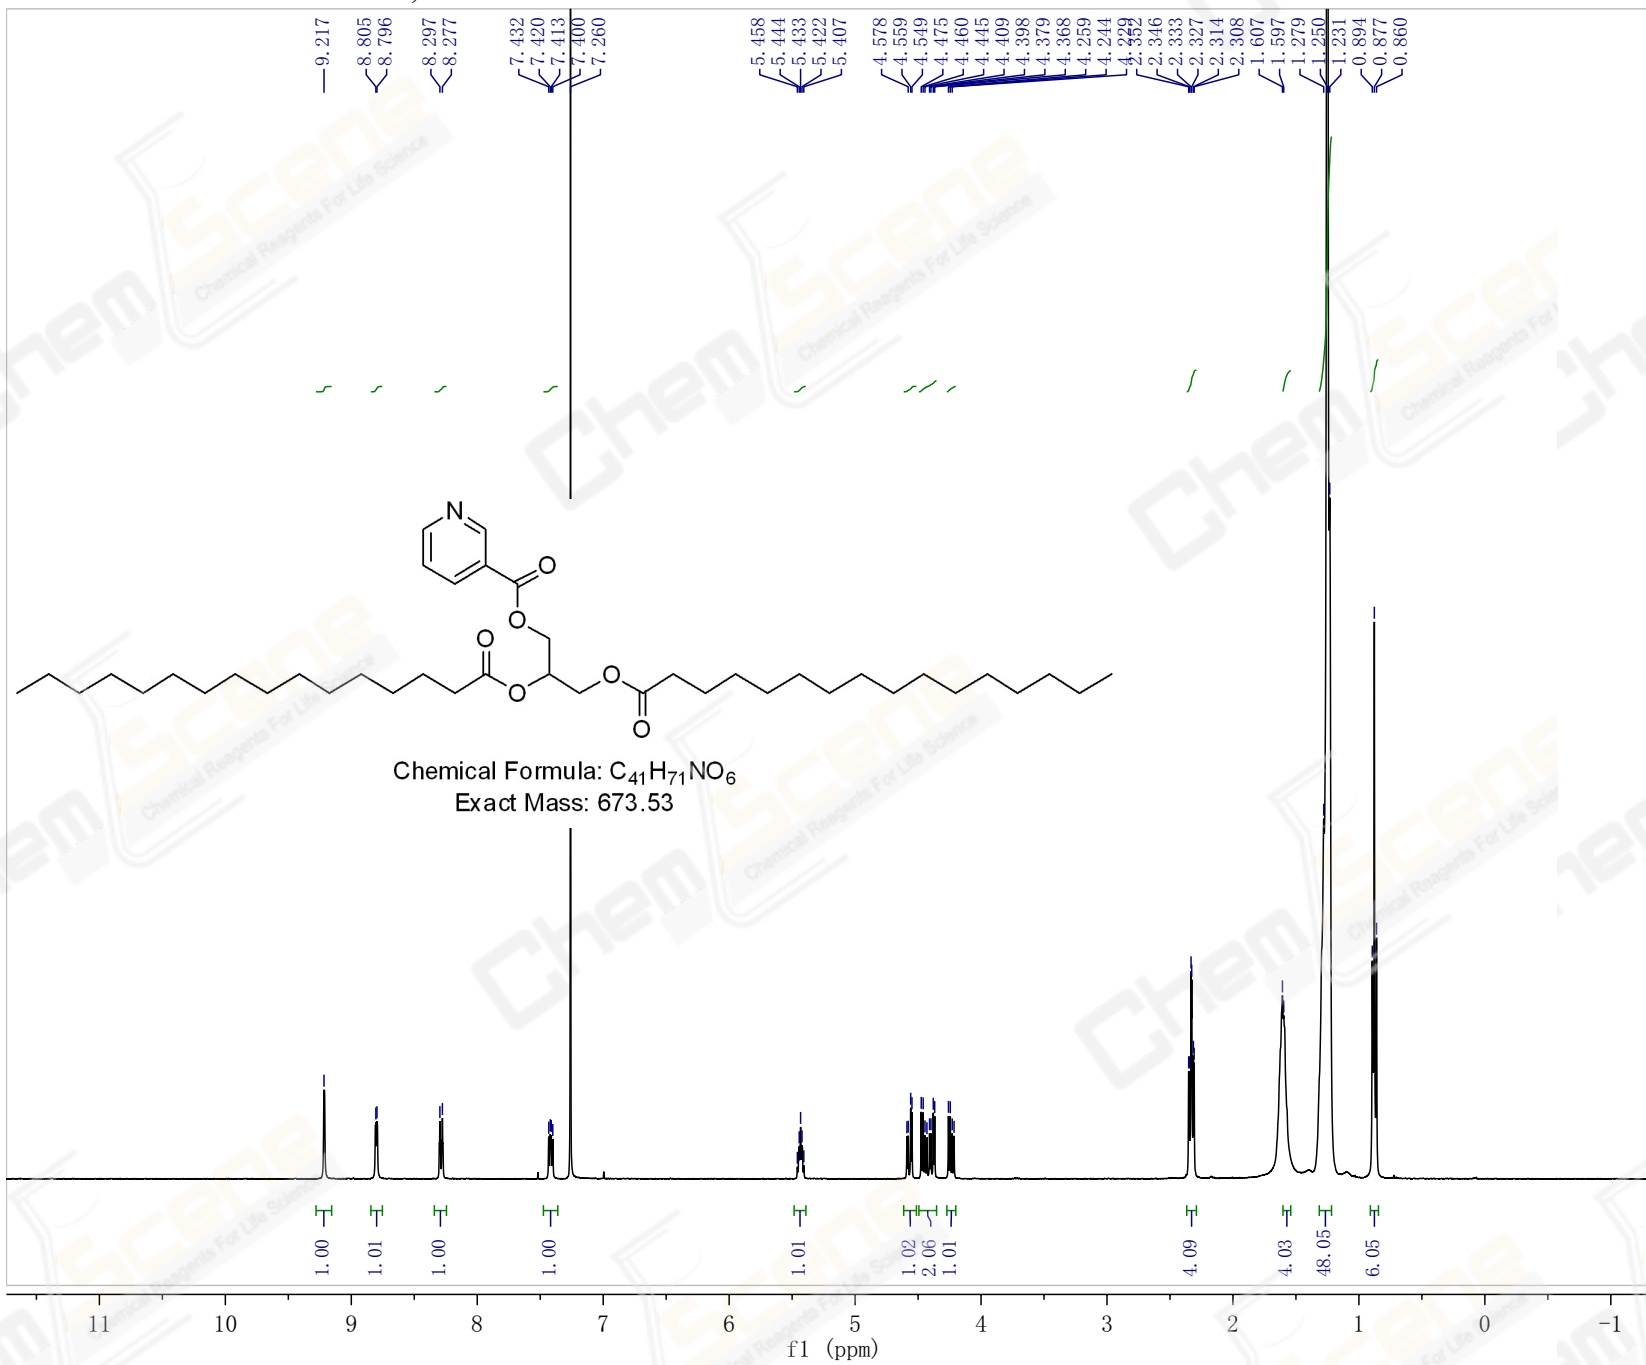

| Parameter | Value |
|---------------------------|---------------------|
| 1 Title | |
| 2 Spectrometer | Avance |
| 3 Solvent | CDCl3 |
| 4 Temperature | 298.1 |
| 5 Pulse Sequence | zg30 |
| 6 Number of Scans | 32 |
| 7 Receiver Gain | 101 |
| 8 Relaxation Delay | 1.0000 |
| 9 Pulse Width | 8.0000 |
| 10 Acquisition Time | 3.9977 |
| 11 Acquisition Date | 2024-05-06T09:27:14 |
| 12 Modification Date | 2024-05-06T09:27:21 |
| 13 Spectrometer Frequency | 400.13 |
| 14 Spectral Width | 8196.7 |
| 15 Lowest Frequency | -1627.6 |
| 16 Nucleus | 1H |
| 17 Acquired Size | 32768 |
| 18 Spectral Size | 65536 |