


Sample ID: BIZ2019-918-SCH5, Catalog No: CS-0022591 Batch#45870 , CDCl3

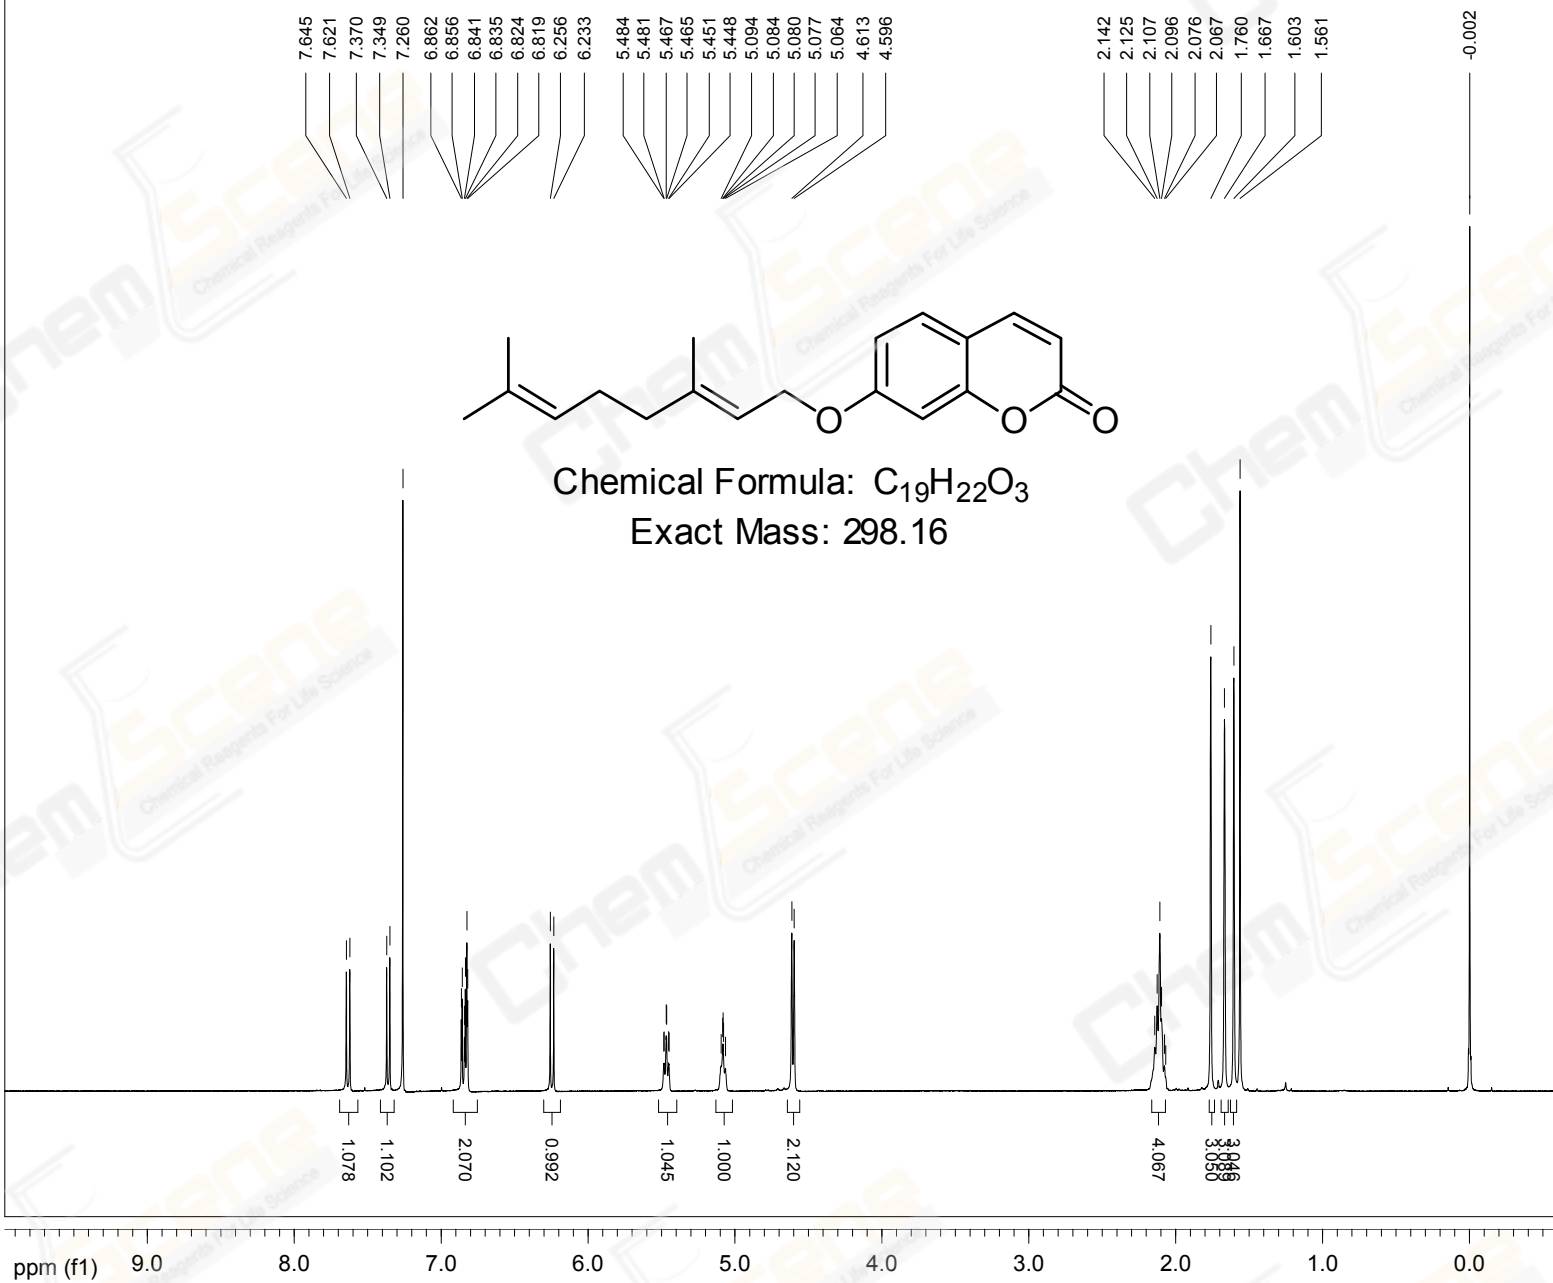

Date:

19 Sep 2019

Document's Title:

Catalog No: CS-0022591 Batch#45870

Spectrum Title:

BIZ2019-918-SCH5-CDCL3-190919

Frequency (MHz):

(f1) 400.132

Original Points Count:

(f1) 26408

Actual Points Count:

(f1) 65536

Acquisition Time (sec):

(f1) 2.9999

Spectral Width (ppm):

(f1) 22.000

Pulse Program:

ZG30

Temperature:

300

Number of Scans:

24

Acq. Date:

Thu Sep 19 02:18:50 PM