


Sample ID: BIZ2019-923-SCH8, Catalog No: CS-4089 Batch#46213, CDCI3

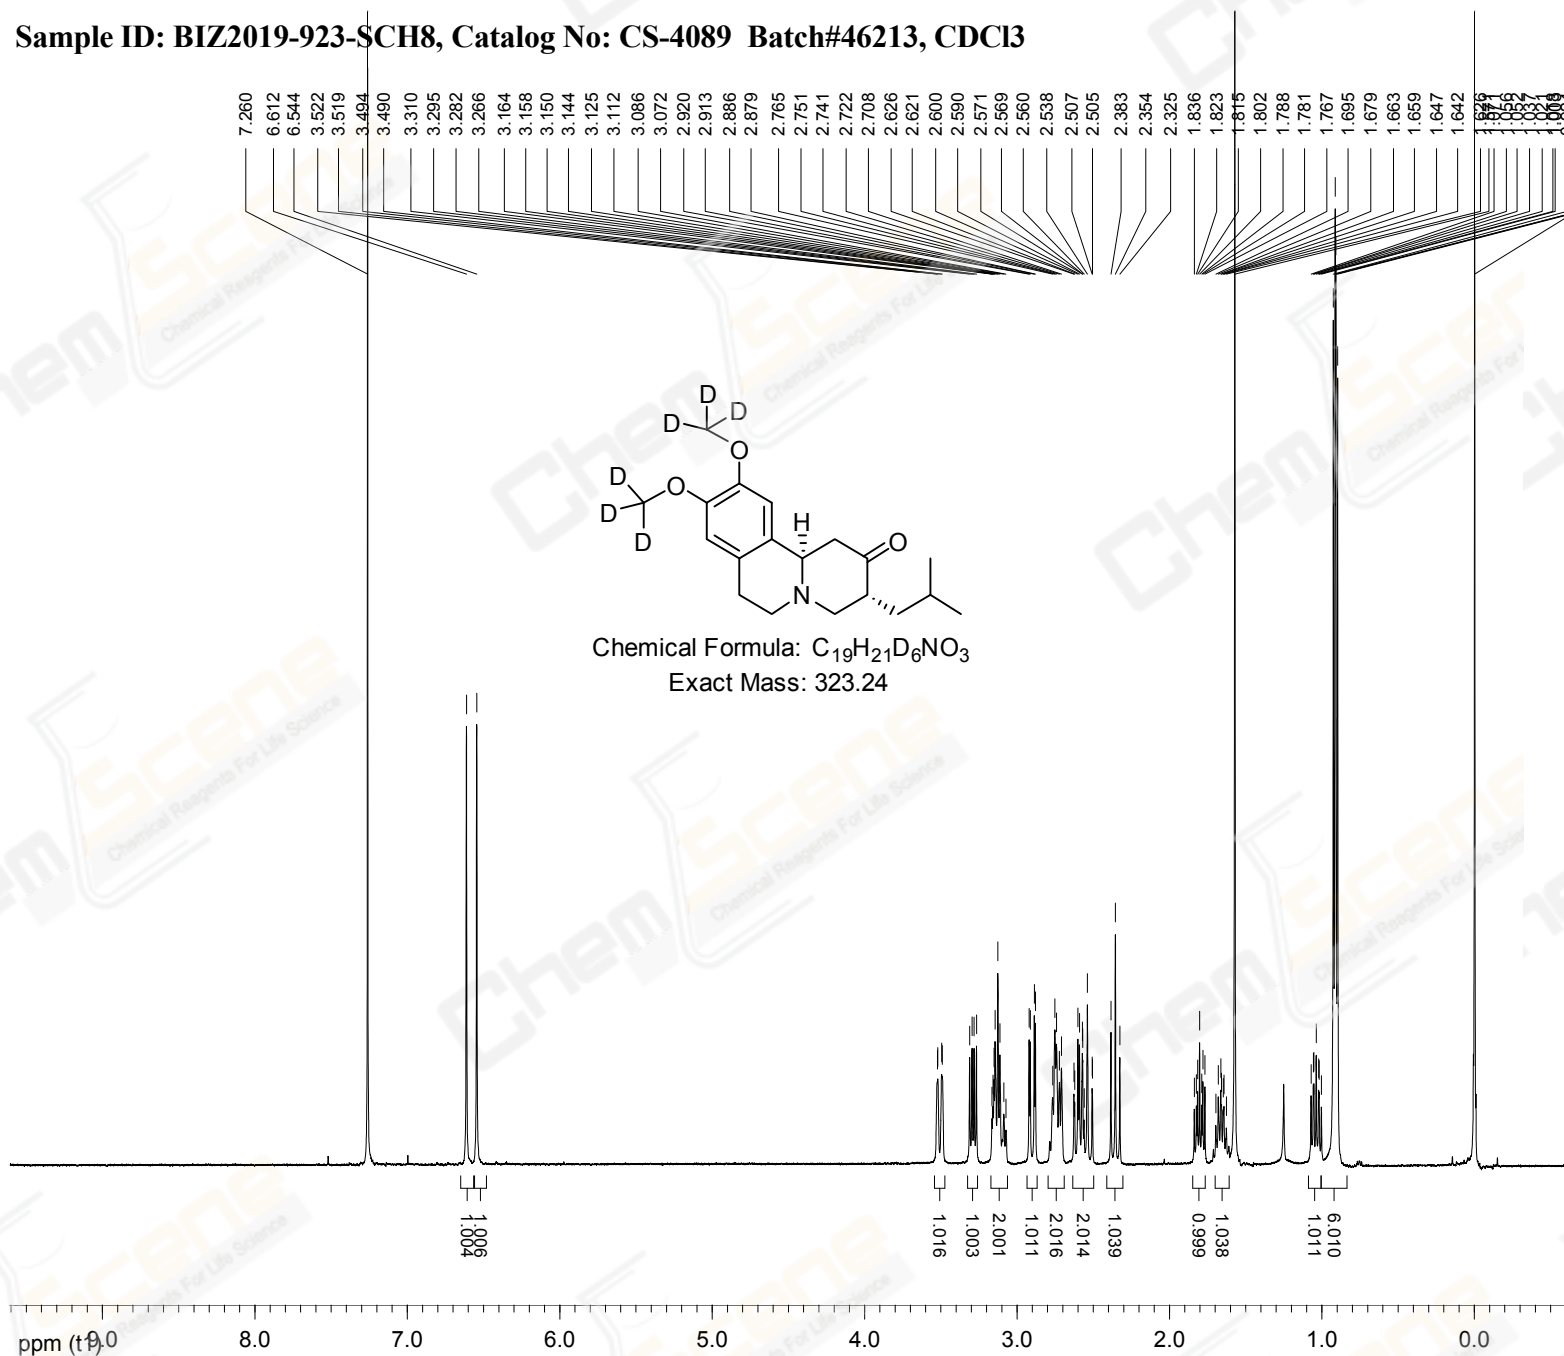

**Date:**  
25 Sep 2019

**Document's Title:**  
Catalog No: CS-4089 Batch#46213

**Spectrum Title:**  
BIZ2019-923-SCH8-CDCL3-190924

**Frequency (MHz):**  
(f1) 400.132

**Original Points Count:**  
(f1) 26408

**Actual Points Count:**  
(f1) 65536

**Acquisition Time (sec):**  
(f1) 2.9999

**Spectral Width (ppm):**  
(f1) 22.000

**Pulse Program:**  
ZG30

**Temperature:**  
300

**Number of Scans:**  
16

**Acq. Date:**  
Tue Sep 24 02:02:10 PM