


Catalog No: CS-3560,CDCL3

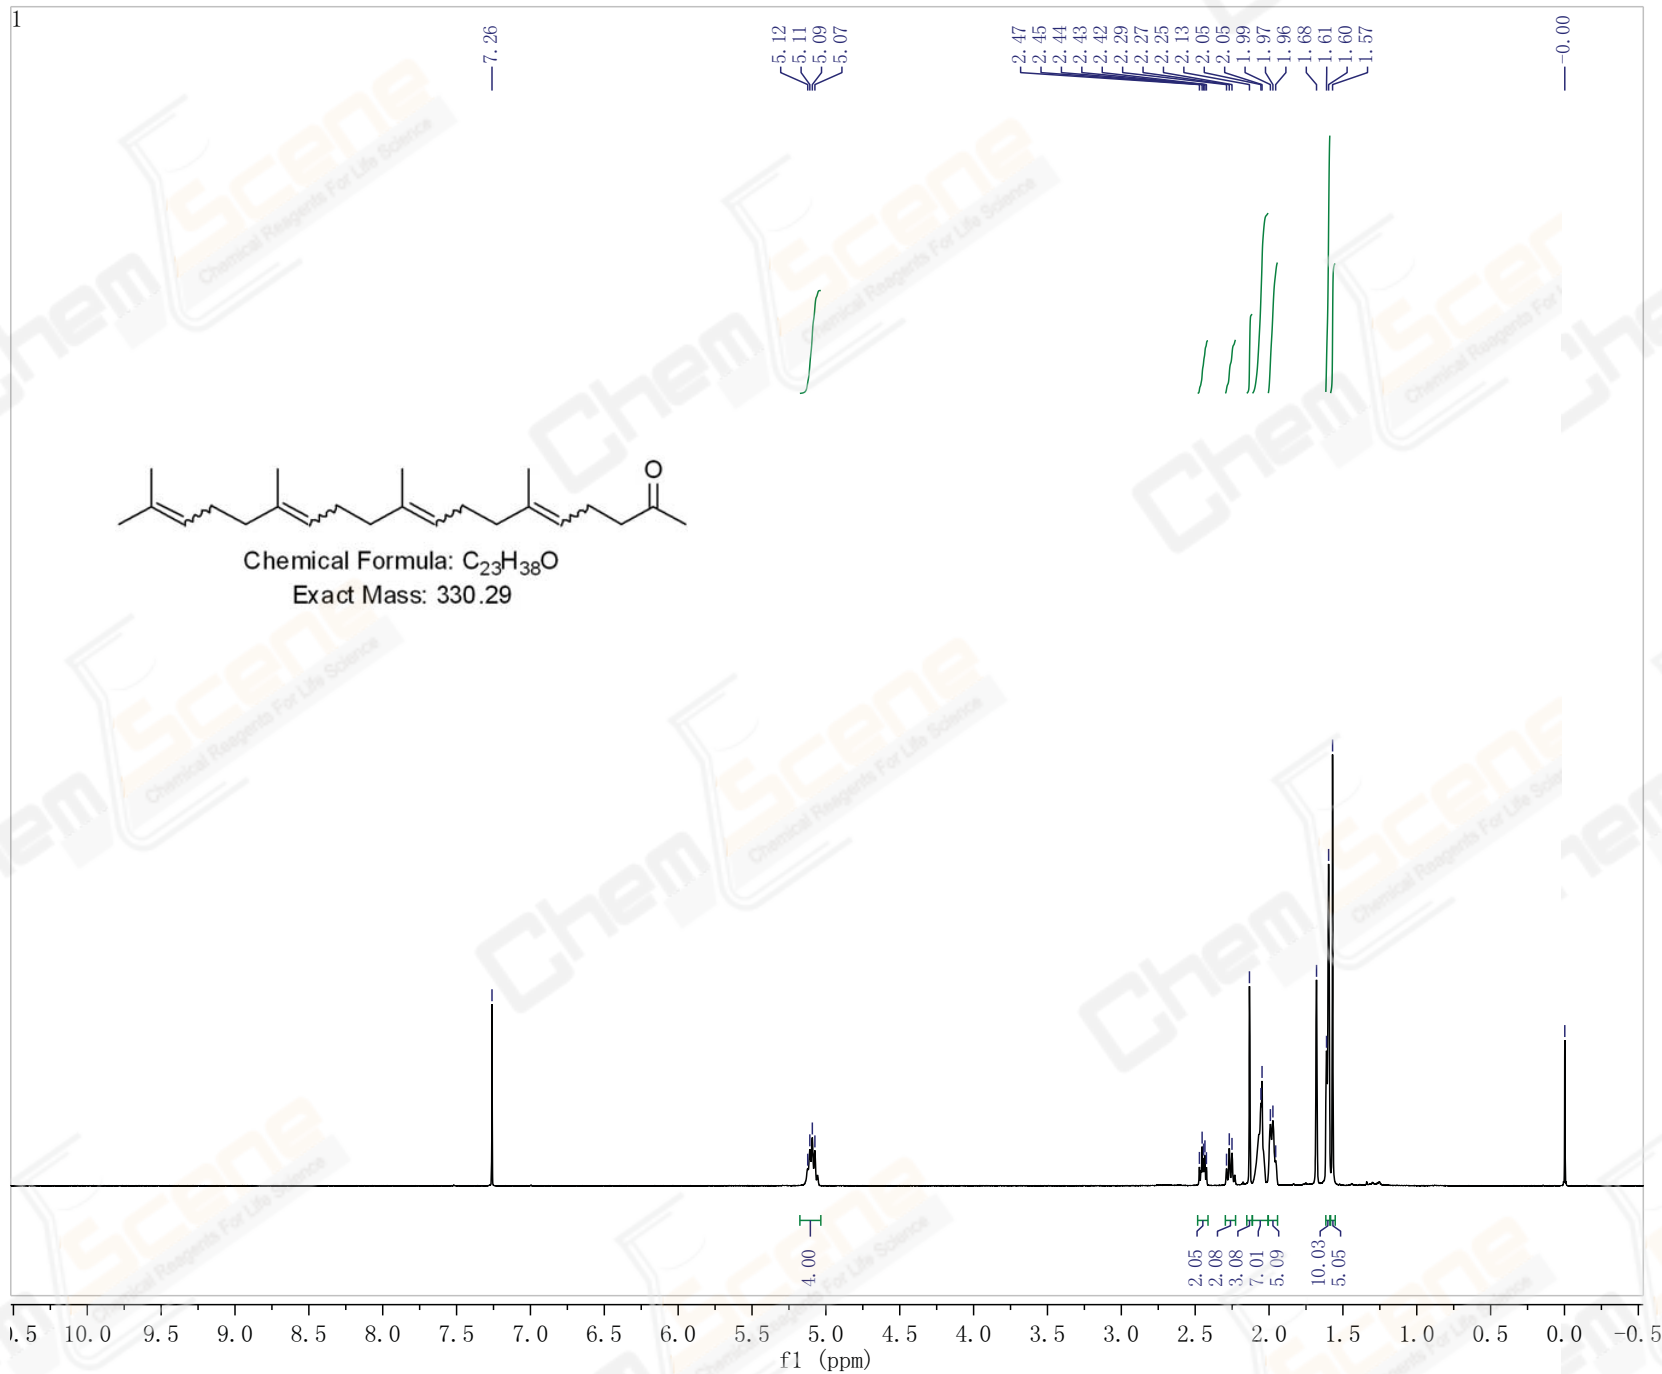

| Parameter | Value |
|---------------------------|---------------------|
| 1 Title | BIZ2020-628-SCH11 |
| 2 Spectrometer | magnet |
| 3 Solvent | CDCL3 |
| 4 Temperature | 298.1 |
| 5 Pulse Sequence | slpul30 |
| 6 Number of Scans | 64 |
| 7 Receiver Gain | 64 |
| 8 Relaxation Delay | 1.0000 |
| 9 Pulse Width | 9.8000 |
| 10 Acquisition Time | 3.9999 |
| 11 Acquisition Date | 2020-06-29T21:07:26 |
| 12 Modification Date | 2020-06-29T21:26:13 |
| 13 Spectrometer Frequency | 400.00 |
| 14 Spectral Width | 8108.0 |
| 15 Lowest Frequency | -1654.0 |
| 16 Nucleus | 1H |
| 17 Acquired Size | 32431 |
| 18 Spectral Size | 65536 |