


Catalog No: CS-0019978,CDCL3

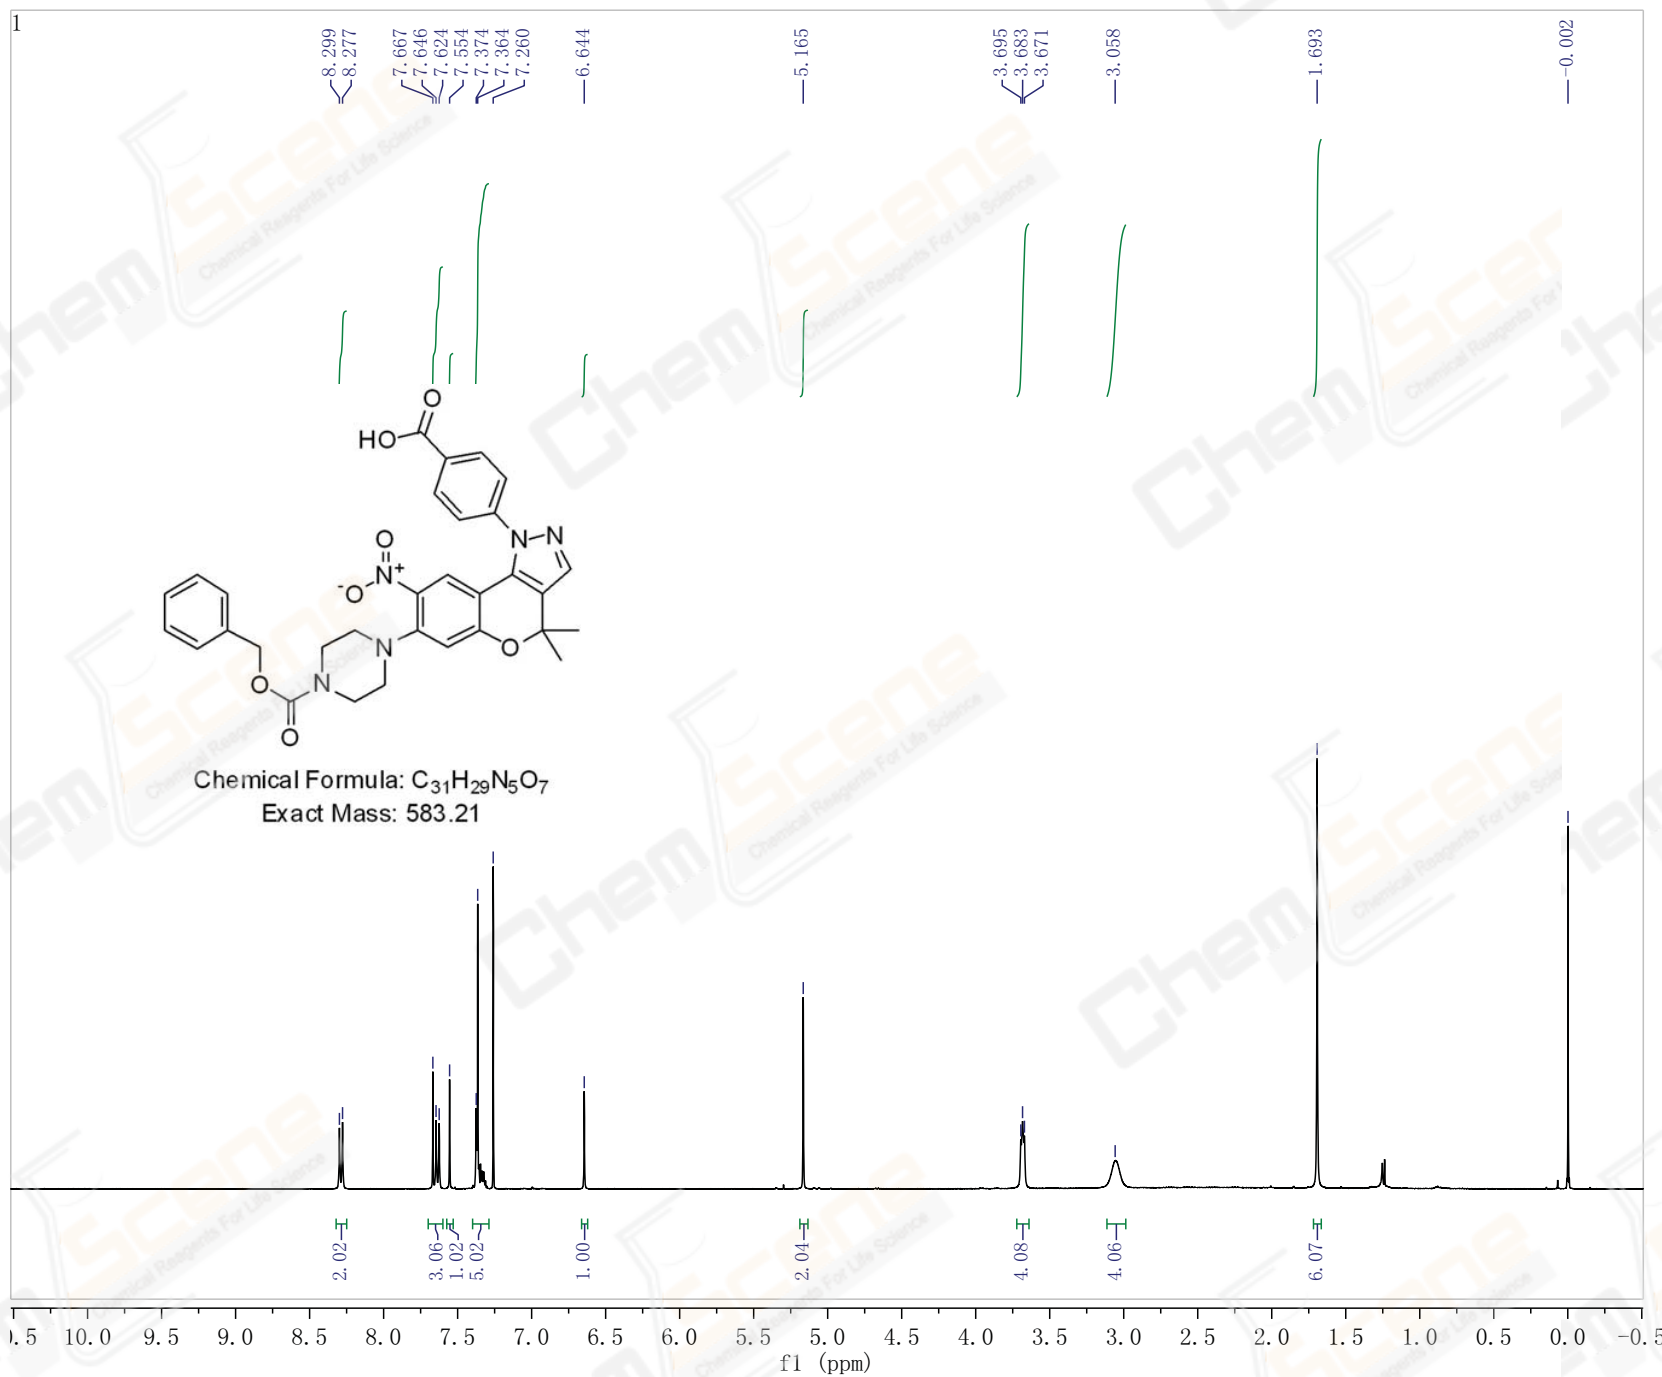

Parameter	Value
1 Title	BIZ2020-910-WLQ6
2 Spectrometer	magnet
3 Solvent	CDCl3
4 Temperature	298.1
5 Pulse Sequence	s1pul30
6 Number of Scans	64
7 Receiver Gain	64
8 Relaxation Delay	1.0000
9 Pulse Width	9.8000
10 Acquisition Time	3.9999
11 Acquisition Date	2020-09-11T19:13:53
12 Modification Date	2020-09-11T19:28:37
13 Spectrometer Frequency	400.00
14 Spectral Width	8108.0
15 Lowest Frequency	-1654.0
16 Nucleus	$^1H$
17 Acquired Size	32431
18 Spectral Size	65536